


Diagnostic-quality acquisition system for bio-electric sensors and bio-impedance measurements

Datasheet - preliminary data

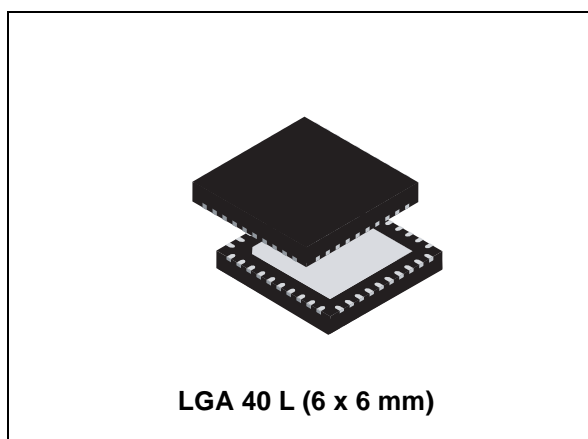

Features

- 3 biopotential acquisition channels with integrated analog high pass filters
- 1 bio-impedance measurement channel with 2- or 4-wire measurement
- Digital IQ demodulation
- Integrated configurable digital filtering and preprocessing
- Pacemaker pulse acquisition with embedded detection function (down to 0.1 mV impulse amplitude)
- Input connection matrix allows support for different cable configurations
- SPI daisy chain supports up to 4 ICs connection
- Programmable analog gain: 8, 16, 32, 64
- Low supply voltage: 1.62 V to 3.6 V
- Input referred noise: 6 μV_{PP} (300 Hz BW, G=64)

- Maximum data rate: 125 kSPS per channel
- Less than 1 mA/channel at full bandwidth and resolution
- DC and AC lead-off detection
- Right leg driver (RLD), Wilson common terminal (WCT) and shield driver (SD)
- Clock reconfigurability
- Built-in ring oscillator ($\pm 5\%$ accuracy)
- Built-in crystal oscillator ($\pm 0.1\%$ accuracy)
- External clock
- Low external component count architecture
- Allows compliance with medical standards ANSI/AAMI EC11, ANSI/AAMI EC13 and IEC60601-2-27
- EMI tolerant

Applications

- ECG (electrocardiogram)
- Carts for clinical environments
- Bedside monitoring
- Holter monitors
- Automated external defibrillator (AED)
- EEG (electroencephalogram)
- EMG (electromyography)
- Wearable remote monitoring
- Medical equipment

Table 1. Device summary

Order code	Biopotential channels	Bio-impedance channel	Marking	Package	Packaging
HM301DL	3	Yes	HM301D	LGA 6x6 40L	Tray

Contents

- 1 Description 7**
- 2 Block diagram 8**
- 3 Pin configuration 9**
- 4 Maximum ratings 11**
- 5 Electrical characteristics 12**
- 6 Detailed description 16**
 - 6.1 Overview 16
 - 6.2 Input connection matrix 17
 - 6.3 Biopotential channel 18
 - 6.3.1 Analog section 18
 - 6.3.2 Digital section 20
 - 6.3.3 High resolution low bandwidth signal path (HRLB) 21
 - 6.3.4 Low resolution high bandwidth signal path (LRHB) 21
 - 6.4 Lead off detection 22
 - 6.4.1 DC contact check 23
 - 6.4.2 AC contact check 23
 - 6.5 Impedance channel 24
 - 6.5.1 Analog section 25
 - 6.5.2 Digital section 25
 - 6.6 Drivers 26
 - 6.6.1 Right leg driver 27
 - 6.6.2 Shield driver 27
 - 6.6.3 Wilson common terminal (WCT) 27
 - 6.7 TM and RST pin configuration 28
 - 6.8 Digital machine 29
 - 6.8.1 Operating modes 29
 - 6.8.2 Sleep 29
 - 6.8.3 Boot 29
 - 6.8.4 Standby 29

6.8.5	Ready	30
6.8.6	Measure	30
6.8.7	Fast recovery	31
6.9	GPIO configuration	32
6.10	SPI interface	36
6.10.1	SPI read	36
6.10.2	SPI write	37
6.10.3	Daisy chain SPI	38
6.10.4	SPI timing	41
6.11	Power supply voltage monitor	42
6.12	Registers MAP	42
6.12.1	Application settings (Read/Write)	46
6.12.2	Output flags (read only)	60
6.12.3	Data registers (readable only if MEAS_MODE = 1)	61
6.13	Output data format	69
6.13.1	Case 1: complete processed data - 4x packet	70
6.13.2	Case 2: pre-filtered data out - 3x packet	71
6.13.3	Header description	72
6.14	Data rate	74
6.15	Data ready operation	75
7	Application Information	77
7.1	DC offset removal	77
7.2	Multi-chip configuration	78
7.3	Supported ECG configurations	80
8	Package mechanical data	81
9	Revision history	84

List of tables

Table 1.	Device summary	1
Table 2.	Pin description	9
Table 3.	Absolute maximum ratings	11
Table 4.	Thermal data	11
Table 5.	Electrical characteristics	12
Table 6.	Input-referred noise ($\mu\text{V}_{\text{RMS}}/\mu\text{V}_{\text{PP}}$) / 3 V analog supply 1	15
Table 7.	Input connection matrix	17
Table 8.	Pad connection settings	18
Table 9.	Biopotential channel gain and IDR	19
Table 10.	Functional modes	29
Table 11.	Digital GPIO output signals (DGIO0)	32
Table 12.	Digital GPIO output signals (DGIO1)	33
Table 13.	Digital GPIO output signals (DGIO2)	34
Table 14.	Digital GPIO input signals	36
Table 15.	Read command bytes	37
Table 16.	Write command byte	38
Table 17.	SPI slave timings (IOVDD = 1.8 V)	41
Table 18.	Psmon_out signal	42
Table 19.	Registers MAP	42
Table 20.	Registers MAP	44
Table 21.	Data registers (readable only if meas_mode bit is 1)	45
Table 22.	SET0 CH_ENABLE (ADDR 27h)	46
Table 23.	SET1 PM_SEL (ADDR 28h)	46
Table 24.	SET 2 AVG_CTRL (ADDR 29h)	47
Table 25.	SET3 INCON_HCSEL_1 (2Ah)	47
Table 26.	SET4 INCON_HCSEL_2 (2Bh)	48
Table 27.	SET5 INCON_HCSEL_3 (2Ch)	48
Table 28.	SET6 INCON_AVG_1 (2Dh)	48
Table 29.	SET7 INCON_AVG_2 (2Eh)	49
Table 30.	SET8 INCON_RLD (2Fh)	49
Table 31.	SET9 CCK_EN_1 (30h)	50
Table 32.	SET10 CCK_EN_2 (31h)	50
Table 33.	SET11 CCK_CUR (32h)	51
Table 34.	SET12 CCK_TRSH (33h)	52
Table 35.	SET13 HC_ANA_CTRL (34h)	53
Table 36.	SET14 IMP_ANA_CTRL (35h)	53
Table 37.	SET15 ECG_DIGFILT_CTRL (36h)	54
Table 38.	SET16 PM_DIGFILT_CTRL (37h)	54
Table 39.	SET17 HC_DIGFILT_CTRL (38h)	55
Table 40.	SET18 HC_HPFANA_CTRL (39h)	55
Table 41.	SET19 RLD_CTRL (3Ah)	56
Table 42.	SET20 RECOVERY_TIME (3Bh)	57
Table 43.	SET21 PMD_TRSH (3Ch)	57
Table 44.	SET22 FILTER_SWTIME (3Dh)	58
Table 45.	SET23 DIGIO_IO (40h)	58
Table 46.	SET24 IMP_CUR_EN (44h)	58
Table 47.	SET25 DIGIO12_SEL (45h)	59
Table 48.	SET26 DIGIO0_SEL (46h)	59

Table 49.	OUT_FLAG0 (47h)	60
Table 50.	OUT_FLAG1 (48h)	60
Table 51.	ECG1_DATAOUT_1 (49h)	61
Table 52.	CG1_DATAOUT_0 (4Ah)	61
Table 53.	ECG2_DATAOUT_1 (4Bh)	61
Table 54.	ECG2_DATAOUT_0 (4Ch)	62
Table 55.	ECG3_DATAOUT_1 (4Dh)	62
Table 56.	ECG3_DATAOUT_0 (4Eh)	62
Table 57.	ECG12_DATAOUT_1 (4Fh)	63
Table 58.	ECG12_DATAOUT_0 (50h)	63
Table 59.	ECG23_DATAOUT_1 (51h)	63
Table 60.	ECG23_DATAOUT_0 (52h)	64
Table 61.	ECG31_DATAOUT_1 (53h)	64
Table 62.	ECG31_DATAOUT_0 (54h)	64
Table 63.	PM1_DATAOUT_1 (55h)	65
Table 64.	PM1_DATAOUT_0 (56h)	65
Table 65.	PM2_DATAOUT_1 (57h)	65
Table 66.	PM2_DATAOUT_0 (58h)	66
Table 67.	IMPEDANCE_PHASE_AC_DATAOUT_1 (59h)	66
Table 68.	IMPEDANCE_PHASE_AC_DATAOUT_0 (5Ah)	66
Table 69.	IMPEDANCE_SQUARING_AC_DATAOUT_1 (5Bh)	67
Table 70.	IMPEDANCE_SQUARING_AC_DATAOUT_0 (5Ch)	67
Table 71.	IMPEDANCE_PHASE_DC_DATAOUT_1 (5Dh)	67
Table 72.	IMPEDANCE_PHASE_DC_DATAOUT_0 (5Eh)	68
Table 73.	IMPEDANCE_SQUARING_DC_DATAOUT_1 (5Fh)	68
Table 74.	IMPEDANCE_SQUARING_DC_DATAOUT_0 (60h)	68
Table 75.	CONTACT_CHECK_DATAOUT_1 (61h)	69
Table 76.	CONTACT_CHECK_DATAOUT_0 (62h)	69
Table 77.	Data format	70
Table 78.	Base pocket	70
Table 79.	Data packet out with 3 HM301D in chain	70
Table 80.	Pre-filtered data out	71
Table 81.	Header packet bits description in 4x packet case	72
Table 82.	Header packet bits description in 3x packet case	72
Table 83.	C_DATA packet description bits configurations	73
Table 84.	Contact check and overflow C_DATA vector	73
Table 85.	HRLB data-out sampling frequency vs low pass filter cut-off frequency	74
Table 86.	LRHB data-out sampling frequency vs low pass filter cut-off frequency	74
Table 87.	Impedance data-out sampling frequency vs low pass filter cut-off frequency	75
Table 88.	Common ECG configurations	80
Table 89.	LGA 40L (6 x 6 mm) mechanical data	83
Table 90.	Document revision history	84

List of figures

Figure 1.	HM301D block diagram	8
Figure 2.	Pin configuration (top view)	9
Figure 3.	Biopotential channel block schematic	18
Figure 4.	First decimation filter	20
Figure 5.	HRLB digital signal path	21
Figure 6.	LRHB signal path	22
Figure 7.	Contact check architecture	23
Figure 8.	Impedance channel architecture	24
Figure 9.	Impedance channel digital section	26
Figure 10.	AVG buffers	27
Figure 11.	WCT buffer	28
Figure 12.	State machine for packets streaming mode (meas_mode = 0)	30
Figure 13.	State machine for packets streaming mode (meas_mode = 1)	31
Figure 14.	Single byte reading	37
Figure 15.	Double byte reading	37
Figure 16.	Single byte writing	38
Figure 17.	Example of daisy chain SPI connection with 3 HM301D	38
Figure 18.	Example of daisy chain SPI writing	39
Figure 19.	Example of daisy chain SPI reading	40
Figure 20.	SPI timing	41
Figure 21.	SPI communication - packet data streaming	75
Figure 22.	ECG_OUT registers data reading	76
Figure 23.	Maximum DC offset removal	78
Figure 24.	Example of chain connection: standard 12-lead ECG	79
Figure 25.	Package outline for LGA 40L (6 x 6 mm)	82

1 Description

The HM301D is a highly integrated diagnostic-quality biopotential acquisition system with 3 differential channels. Multi master/slave configuration supports up to 16 channels of simultaneous sampling (12 biopotential acquisitions and 4 bio-impedance channels). A fully integrated high-pass filter removes the half-cell DC value to enable the channels to work with the AC component only. Each channel provides high resolution and low noise conversion of biopotential signals up to 10 kHz.

The input connection circuit matrix guarantees maximum flexibility in terms of electrode cables and connectors.


The HM301D includes a dedicated impedance measurement channel that can be used to measure both body impedance average value and variation due to respiration. This channel delivers both the real and the imaginary parts of the body and the breathing impedances. The WCT circuit and driver block implements the driving functions (right leg driver and shield driver) and the Wilson common terminal commonly used in ECG systems.

The electrode-to-skin contact is checked by injecting an AC or DC current. A digital filtering and preprocessing (DFP) block implements configurable band-pass filters, IQ impedance demodulation and enables specific algorithm implementation for lead-off check and pacemaker detection.

The SPI interface allows the exchange of data with both the microcontroller and other HM301D devices in case of chain connection. Full configurability and low power design techniques make it ideal for many applications, including battery-powered devices. High quality recordings are obtained with a small, power-saving system. The 3-channel version is available in a 6 x 6 mm 40-lead LGA.

2 Block diagram

Figure 1. HM301D block diagram

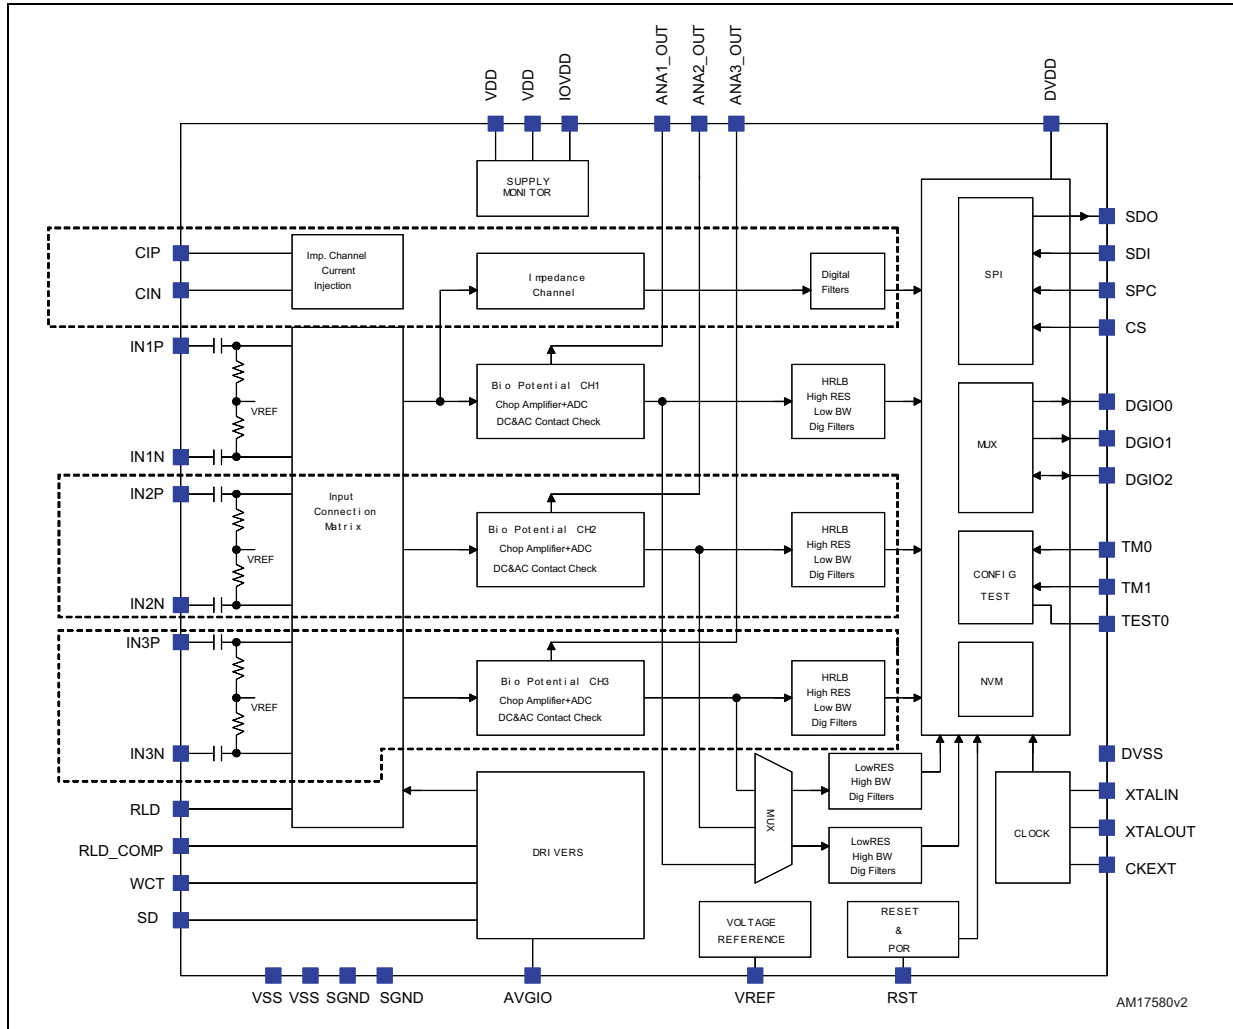

3 Pin configuration

Figure 2. Pin configuration (top view)

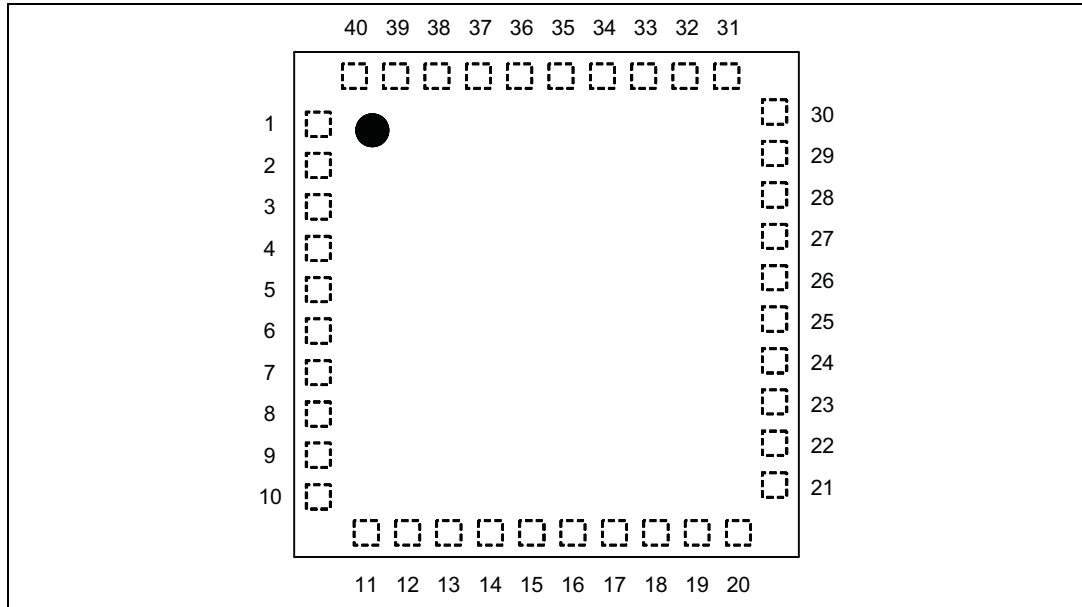


Table 2. Pin description

Pin name	Pin n°	Type	Description
IN1P	1	ANA IN	Connected to biopotential channel #1 positive input by default. See <i>input connection matrix</i> to change it
IN1N	2	ANA IN	Connected to biopotential channel #1 negative input by default. See <i>input connection matrix</i> to change it
VDD	3	ANA IN	Analog supply voltage
IN2P	4	ANA IN	Connected to biopotential channel #2 positive input by default. See <i>input connection matrix</i> to change it
IN2N	5	ANA IN	Connected to biopotential channel #2 negative input by default. See <i>input connection matrix</i> to change it
VSS	6	ANA GND	Analog ground
IN3P	7	ANA IN	Connected to biopotential channel #3 positive input by default. See <i>input connection matrix</i> to change it
IN3N	8	ANA IN	Connected to biopotential channel #3 negative input by default. See <i>input connection matrix</i> to change it
RLD	9	ANA OUT	Connected to Right Leg Driver output by default. See <i>input connection matrix</i> to change it
WCT	10	ANA OUT	Wilson Common Terminal output
RLD_COMP	11	ANA IO	Input of RLD buffer. To be used for compensation in case of instability of RLD loop

Table 2. Pin description (continued)

Pin name	Pin n°	Type	Description
AVGIO	12	ANA IO	Average value of electrode signals connected to ASSP (O) or coming from other chain connected ASSPs (I)
SD	13	ANA OUT	Driver output of shield cables
ANA1_OUT	14	ANA OUT	Channel1 single ended analog output
ANA2_OUT	15	ANA OUT	Channel2 single ended analog output
ANA3_OUT	16	ANA OUT	Channel3 single ended analog output
TEST0	17	ANA IO	Used for TEST purposes. Leave float in normal operation
VSS	18	ANA GND	Analog ground
VDD	19	ANA IN	Analog supply voltage
VREF	20	ANA IO	Reference voltage to or from other chain connected ASSPs
XTALOUT	21	ANA OUT	Crystal pin connection
XTALIN	22	ANA IN	Crystal pin connection
SGND	23	ANA GND	Analog ground
DVDD	24	ANA IN	Digital supply voltage
CKEXT	25	DIG IO	Clock signal to/from other devices
RST	26	DIG OUT	POR (when TM0 = TM1 = 0)
		DIG IN	Enable (when TM0 = 1, TM1 = 0)
TM0	27	DIG IN	Configuration pin # 1
TM1	28	DIG IN	Configuration pin # 2
DVSS	29	DIG GND	Digital ground
SDO	30	DIG OUT	SPI Serial Data Output
IOVDD	31	ANA IN	Supply voltage for IO pins. It provides the voltage to SPI and GPIOs it must be always lower than VDD.
SDI	32	DIG IN	SPI Serial Data Input
CS	33	DIG IN	SPI Chip Select
SPC	34	DIG IN	SPI Serial Port Clock
DGIO2	35	DIG IO	General purpose digital IO
DGIO1	36	DIG IO	General purpose digital IO
DGIO0	37	DIG IO	General purpose digital IO
SGND	38	ANA GND	Analog ground
CIN	39	ANA OUT	AC Current Injection Negative pin for Impedance Measurement
CIP	40	ANA OUT	AC Current Injection Positive pin for Impedance Measurement

4 Maximum ratings

Table 3. Absolute maximum ratings

Symbol	Parameter	Value ⁽¹⁾	Unit
V _{DD}	Analog Supply Voltage	-0.3 to 4.8	V
DV _{DD}	Digital Supply Voltage	-0.3 to 4.8	V
IOV _{DD}	IOs supply voltage	-0.3 to 4.8	V
Analog I/O	All analog IOs	-0.3 to 4.8	V
Digital I/O	All digital IOs	-0.3 to 4.8	V
T _{OP}	Operating temperature range	-40 to 100	°C
T _{ST}	Storage Temperature Range	-65 to 150	°C
T _J	Maximum Junction Temperature	+150	°C
ESD	HBM	±2	kV
	CDM	500	V

1. All values are referred to VSS.

Note: Absolute maximum ratings are those values beyond which damage to the device may occur. Functional operation under these conditions is not implied.

Table 4. Thermal data

Symbol	Parameter	Value	Unit
R _{THJA}	Junction to ambient thermal resistance	55	°C/W

5 Electrical characteristics

$T_A = 0$ to $70\text{ }^\circ\text{C}$, $V_{DD} = DV_{DD} = IOV_{DD} = 3\text{ V}$, $V_{REF} = 0.7\text{ V}$, unless otherwise specified.

Table 5. Electrical characteristics

Symbol	Parameter	Test conditions	Min.	Typ.	Max	Unit
General section						
AV_{DD} IOV_{DD} DV_{DD}	Supply voltages		1.62		3.6	V
I_{DD}	Current consumption	Power down mode		10		μA
		3 channels ON, Impedance OFF, RLD ON, WCT ON		3	3.6	mA
		1 channel ON, Impedance OFF, RLD ON, WCT OFF		1.3	1.6	mA
		1 channel ON, Impedance ON, RLD ON, WCT OFF		2.2	2.7	mA
V_{IH}	High level input voltage	All Inputs	$0.8 \times IOV_{DD}$			V
V_{IL}	Low level input voltage	All inputs			$0.2 \times IOV_{DD}$	V
V_{OH}	High level output voltage	All outputs	$0.9 \times IOV_{DD}$			V
V_{OL}	Low level output voltage	All outputs			$0.1 \times IOV_{DD}$	V
Biopotential channels						
$V_{BIO-DIFF}$	Differential input voltage	Signal bandwidth 0.05 Hz - 10 kHz		$\pm 0.8/\text{GAIN}$		V
	Input impedance Signal bandwidth 0.05 Hz-300 Hz	DC contact check ON	50			M Ω
		DC contact check OFF	50			
	Analog high pass RC filter cut off frequency			0.05		Hz
	Input bias current				10	pA
	Input differential bias current				10	pA
	Gain setting		8, 16, 32, 64			V/V
	Total gain error	INA+PGA+ADC+VREF			± 1	%
	Gain match between channels			31.25	± 0.5	%
	Chopping frequency			31.25		kHz

Table 5. Electrical characteristics (continued)

Symbol	Parameter	Test conditions	Min.	Typ.	Max	Unit
	Total accuracy (quantization, linearity, noise)	$V_{DIFF-PP}=20mV$; GAIN=64; 10Hz		15		μV
	ADC resolution	AC signal only, DC value removed by high-pass filter		16		bits
ODR	Max data rate (internal filters bypassed)	After 1 st decimation filter		125		KSPS
	Input referred noise Signal bandwidth 0.1 Hz - 150 Hz Data rate = 488 Hz	GAIN=64		0.6		μV_{rms}
		GAIN=32		1.1		
		GAIN=16		2		
		GAIN=8		4.2		
CMRR	Common mode rejection ratio	60Hz, 100mV _{PP}		100		dB
SNR	Signal to noise ratio	Gain=64, Differential input signal frequency 10Hz, 10mVpp; VDD=3V HRLB		72		dB
		Gain=16, Differential input signal frequency 1kHz, 40mVpp; VDD=3V LRHB		62		dB
Impedance channel						
$V_{ZC-DIFF}$	Differential input voltage			$\pm 0.8 /$ GAIN		V
	Gain setting		8, 16, 32, 64			V/V
	Accuracy (quantization, linearity, noise)	DC Impedance range [50, 5k] Ω , point calibration 50 Ω		± 1.5		%
	ADC Resolution			16		bits
	Impedance measurement noise	0.05 Hz to 1 Hz filter, 31.25 kHz modulation frequency, 100 Ohm baseline resistance 20 μA with Gain = 64		100		m Ω
	Total phase shift			115		deg
	Gain error				± 0.1	%
Impedance channel current injection						
	Injection current		5, 10, 20			μA
	Sink/Source current matching				15	nA
	Current Injection frequency		31.25			kHz
RLD amplifier						
	Integrated noise	bandwidth 0,05Hz-300Hz		20		μV_{rms}

Table 5. Electrical characteristics (continued)

Symbol	Parameter	Test conditions	Min.	Typ.	Max	Unit
	Gain	f=50Hz	50			dB
	Output voltage swing	ILIM 880 nA	V _{SS} + 0.325		V _{DD} -0.35	V
	Sink/Source current	VDD = 3V			11	µA
	Current consumption			90		µA
WCT amplifier						
	Integrated noise	bandwidth 0,05Hz-300Hz		1.5		µVrms
	Gain bandwidth product		0.5			MHz
	Gain			1		V/V
	Sink/Source current			33/18		µA
	Output voltage swing	V _{DD} =1.8V	V _{REF} -0.5		V _{REF} + 0.5	V
Shield amplifier						
	Integrated Noise	bandwidth 0.05Hz-300Hz		8		µVrms
	Gain			1		V/V
	Bandwidth		490			Hz
	Sink/Source current				10	µA
	Output Voltage Swing	High Level, V _{DD} =1.8V	V _{REF} - 0.63		V _{REF} + 0.59	V
	Current consumption			11		µA
DC contact check						
	DC Current		25, 50, 100, 200			nA
	DC current accuracy	T _A =25°C		±5		%
	Comparator threshold	T _A =25°C	V _{SS} + 102		V _{DD} - 102	mV
	Step threshold			102		mV
AC contact check						
	Injection current		5, 10, 20			µA
	Sink/Source current matching					nA
	Current Injection frequency	See hc_curinj_freq bit	2.5, 5			kHz
Voltage reference						
V _{REF}	Reference voltage	V _{DD} =3.3V; psmon_sel_r=1		1.0		V
	Accuracy	1 point temperature calibration; T _A =25°C			±0.15	%

Table 5. Electrical characteristics (continued)

Symbol	Parameter	Test conditions	Min.	Typ.	Max	Unit
	Integrated noise	bandwidth 0.05Hz-300Hz		15		μVrms
Ring oscillator						
	Frequency			2.00		MHz
	Accuracy	T _A =25°C			±2	%
		T _A =0÷70°C			±10	%
	Current consumption			12		μA
	Duty cycle		40		60	%
Crystal oscillator						
	Frequency	4 MHz Crystal, internally divided by 2		2.00		MHz
	Accuracy	T _A =0÷70°C			±0.1	%
	Current consumption			68		μA
	Duty cycle		40		60	%
External clock						
	Frequency			2.00		MHz
	Low level signal				0.1 x IOVDD	V
	High level signal		0.9 x IOVDD			V
	Duty cycle		40		60	%

Table 6. Input-referred noise (μV_{RMS}/μV_{PP}) / 3 V analog supply 1

Output data rate (Hz)	-3 dB Bandwidth (Hz)	Gain = 8	Gain = 16	Gain = 32	Gain = 64
1953	600	6.2/41.5	3.1/20.2	1.56/11.3	0.931/6.8
976	300	5.2/37	2.7/18.7	1.39/10.1	0.81/6.4
651	200	5.5/36	3.78/22.1	1.3/8.4	0.841/5.3
488	150	4.2/28	1.98/14.4	1.1/7.17	0.615/4.2
325	100	4.0/27.1	3.0/17.7	1.01/6.8	0.715/4.5
244	75	3.1/20	1.7/11.1	0.93/5.87	0.554/3.8
163	50	3.1/19.5	1.59/10.04	0.83/6.1	0.7/3.4
122	37	2.4/15.8	1.2/8.1	0.76/4.5	0.46/2.6
81.5	25	2.5/15.5	1.55/8.39	0.78/4.5	0.47/2.6

6 Detailed description

6.1 Overview

The HM301D includes three biopotential channels with bio-impedance channel. Even if specifically designed for ECG application, the HM301D is suitable to collect any biopotential signal including EEG and EMG ones.

The biopotential channels measure both the incoming ECG/EEG/EMG and pacemaker (PM) signals and provide both analog (on ANAx_OUT pins) and digital (send out over SPI) outputs. An additional feature of each biopotential channel is the contact check whose purpose is to notify the user when the electrode contact has become poor. This is a DC and AC check and gives an indication on the electrode contact resistance.

The architecture of the biopotential channel is described in more detail in [Section 6.3](#).

The bio-impedance channel provides an accurate measurement of the body and electrode impedance. An AC-current is injected at a configurable frequency through the body; the resulting AC-voltage is measured and processed. In order to get rid of the impedance given by the defibrillator protections resistors, a 4 wires measurement (force and sense) can be implemented by connecting two dedicated electrodes to the injection pins (CIP and CIN). [Section 6.5](#) provides more details about the architecture of this channel.

The input connection circuit allows the use of several kinds of cable connectors based on the application. Any of the input signals on INxy, ($x = 1, 2, 3$; $y = P, N$) can be switched to any of the 3 biopotential channel inputs. Also the output of the RLD can be connected to any INxy.

The drivers block (see [Section 6.6](#)) provides specific reference signals required in both standard ECG applications and multiple chip configuration (e.g. WCT, RLD, SD).

The Wilson common terminal circuit (see [Section 6.6.3](#)) averages the signals present on the R,L and LL electrodes and serves as a reference voltage for unipolar measurements (e.g. ECG: V1,V2...V6).

The right leg drive (see [Section 6.6.1](#)) sets a proper DC-voltage at the input of the HM301D by connecting the RLD output to the RL electrode on the body. RLD_COMP pin allows for the use of an external compensation network, if needed. In case of shielded cables a Shield Driver (see [Section 6.6.2](#)) is provided.

In order to enable applications with a large number of electrodes (e.g. R, L, LL, V1, V2, V3, ...) it is possible to use the HM301D in a multiple chip configuration: up to four devices can be connected using a daisy chain SPI. In this case, all the AVGIO pins are tied together in order to provide the overall common mode signal of all system electrodes.

The HM301D contains a dedicated digital signal processing with the following functionalities:

- User configurable signal filtering: low pass and high pass;
- Simultaneous processing of both High Resolution/Low Bandwidth (HRLB) and High Bandwidth/Low resolution (HBLR) signals (e.g. ECG and Pacemaker);
- IQ impedance demodulation (Real and Imaginary part);
- Standard SPI communication;
- Device configuration settings;

The supply monitor gives a 2-bit indication of the battery status. An accurate voltage reference is embedded. The RST pin can be configured to provide a power-on-reset signal or to accept an external enable signal from the MCU.

The clock circuit offers the maximum configurability:

- Embedded ring oscillator;
- Crystal oscillator;
- External clock;

6.2 Input connection matrix

The input connection circuit allows the use of several kinds of connectors. Anyone of the input pins IN_{xy} (x = 1, 2, 3; y = P/N) can be switched to any of the 3 biopotential channel inputs and to the RLD driver output.

Since the signals of the input pins can change according to the connector used, also the connections of the AVG buffers block must be changed. This is done by setting the right bits according to the following table:

Table 7. Input connection matrix

Setting	Description	Default
inputcon_in1p_hcsel_r<2:0>	Connect input pad IN1P to one of the 6 health channel inputs	111
inputcon_in1n_hcsel_r<2:0>	Connect input pad IN1N to one of the 6 health channel inputs	111
inputcon_in2p_hcsel_r<2:0>	Connect input pad IN2P to one of the 6 health channel inputs	111
inputcon_in2n_hcsel_r<2:0>	Connect input pad IN2N to one of the 6 health channel inputs	111
inputcon_in3p_hcsel_r<2:0>	Connect input pad IN3P to one of the 6 health channel inputs	111
inputcon_in3n_hcsel_r<2:0>	Connect input pad IN3N to one of the 6 health channel inputs	111
inputcon_avg1_r<2:0>	Connect input AVG buffer1 to any of the 6 input pads IN _{xy} (x=1,2,3;y=P/N)	111
inputcon_avg2_r<2:0>	Connect input AVG buffer2 to any of the 6 input pads IN _{xy} (x=1,2,3;y=P/N)	111
inputcon_avg3_r<2:0>	Connect input AVG buffer3 to any of the 6 input pads IN _{xy} (x=1,2,3;y=P/N)	111
inputcon_avg4_r<2:0>	Connect input AVG buffer4 to any of the 6 input pads IN _{xy} (x=1,2,3;y=P/N)	111
inputcon_rld_sel_r<2:0>	Connect the RLD out to any of the inputs pads IN _{xN/P} , for x=1,2,3. Whatever is the bits configuration, the RLD out is always connected to RLD pin.	111

For all the registers the following configuration is valid:

Table 8. Pad connection settings

Bits configuration	Pad connection
000	IN1P
001	IN1N
010	IN2P
011	IN2N
100	IN3P
101	IN3N
110	NOT CONNECTED
111	NOT CONNECTED

The nomenclature used in the pin description and pin configuration is referred to the default setting of the connection matrix. The RLD driver output can be connected to any of the INxy pads but, in any case, it is always connected to RLD pin.

6.3 Biopotential channel

Figure 3. Biopotential channel block schematic

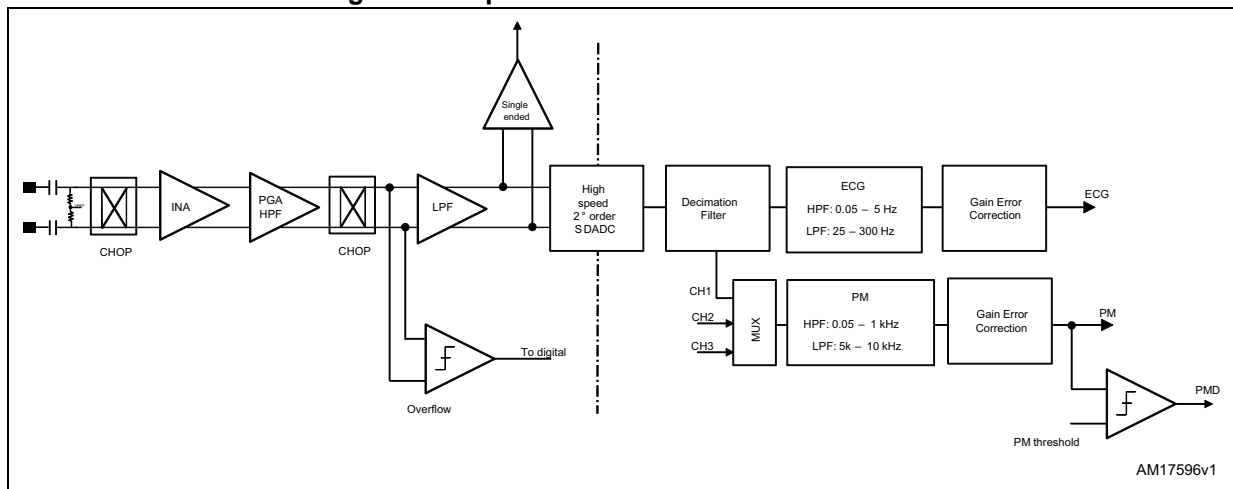


Figure 3 shows the architecture of one biopotential channel. Each channel can be selectively switched on/off.

The high resolution low bandwidth signal is available in ECGx_DATAOUT registers while the a low resolution high bandwidth signal is available in the output data packet.

6.3.1 Analog section

The input signal first passes through the analog high-pass filter with corner frequency of 0.05 Hz, in this way the DC component is removed maintaining the integrity of the signal even at low frequencies.

Due to the very low cut-off frequency, the start-up time of the channel could be very long. In order to avoid this, the HM301D goes in recovery mode in which the high pass filter cut-off frequency is changed to higher values.

At start-up or after overvoltage condition, the cut-off starts from 5 Hz, then goes to 0.7 Hz and finally to 0.05 Hz. The 5 Hz cut-off frequency has a very fast settling speed and will set the common mode level of the instrumentation amplifier. By default, the switching time between the different cut-off frequencies is set at 200 ms but it can be changed in the SET22 register. The recovery mode acts both on analog and digital high pass filters, but the digital filter stops at the frequency which has been set in the hc_dig_pmhpf_sel_r bits.

If the recovery mode is OFF, the cut off frequency of this analog high pass filter can be changed at application level by changing the hc[1,2,3]rhpf_sel_r bits.

After the high pass filter, the signal is chopped and fed to the amplification stage (instrumentation amplifier and programmable gain amplifier). The signal is filtered by a 110 kHz low pass before being supplied to the ADC.

A differential to single-ended block makes the analog signal available at the pins ANA[1,2,3]_OUT. The output voltage of the differential to single-ended block is equal to:

Equation 1

$$DIFF\ 2SE_OUT = GAIN \times \frac{V_{INxP} - V_{INxN}}{2} + V_{REF}$$

where V_{REF} is 0.7 V or 1 V

Table 9. Biopotential channel gain and IDR

IA GAIN	PGA GAIN	IDR [mv]
8	1	200
8	2	100
16	2	50
16	4	25

The ADC is a 2nd order 16bits $\Sigma\Delta$ working at 2 MHz. Since the DC component of the signal has been already removed by the high-pass filter, the ADC is sampling just the useful part of the signal so that the 16bits provide a very good resolution for any biopotential signal.


The bit stream is then processed in the digital domain.

The following parameters of the analog portion of the biopotential channel can be modified through the SPI interface:

- IA Gain: 8, 16 (hc_ina_gain_r);
- PGA Gain: 1, 2, 4 (hc_pga_gain_r);
- Chopping frequency: 31.2 kHz;
- Cut-off frequency of the analog high pass filter (hc[1,2,3]rhpf_sel_r);

6.3.2 Digital section

Figure 4. First decimation filter

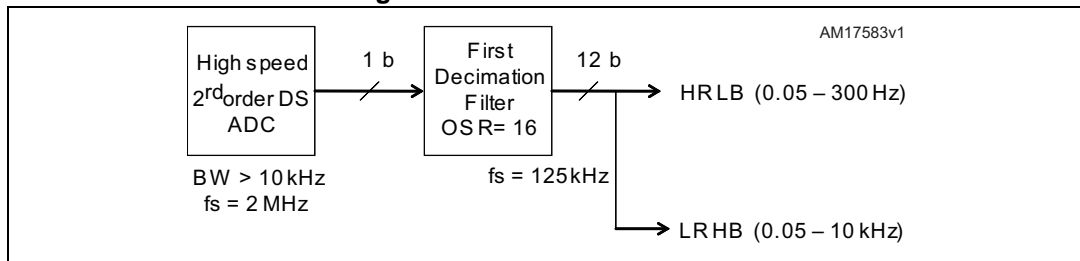

The channel converts two signals to the digital domain: a high resolution low bandwidth (HRLB) and a low resolution high bandwidth (LRHB), for example the ECG and the pacemaker signals respectively. Their frequency content is 0.05-300 Hz and 0.05-10 kHz. While the HRLB are available for all the three biopotential channels, there are two LRHB signal paths which can be connected to any of the three biopotential channels. This is configured through the `pmd_sel_r` bits.

For both HRLB and LRHB signals, the digitized data values are in binary one's complement format. The analog input value is calculated according to the following formula:

Equation 2

$$V_{INxP} - V_{INxN} = \pm \frac{V_{REF}}{GAIN} \cdot \frac{DATA_{10}}{2^{16-1}}$$


where

- SIGN is plus if MSB is 0, minus if MSB is 1;
- DATA10 is the decimal value of the 15 LSBs if MSB is 0 or of the 15bits one's complement if MSB is 1;
- $V_{REF} = 0.8$ V;
- $GAIN = IA_GAIN \times PGA_GAIN$ is the total gain;

The first digital block is a decimation filter. Starting from the 2 MHz 1bit stream provided by the $\Sigma\Delta$ modulator, a decimation rate of 16 is taken. The first decimation stage is then used for both the two signal paths. The sampling frequency is 2 MHz and the output is a 125 kHz 12 bits digital signal. Since the ADC is implemented as a 2nd order delta-sigma, the digital stream has 2nd order noise shaping. This must be filtered adequately to prevent aliasing. To obtain this, a 3rd order CIC-filter was chosen. This filter has an attenuation of -0.274 dB (3%) at 10 kHz and -0.2 m dB at 300 Hz. The output word length is 12 bit which can be provided to the SPI interface by configuring the `bit_dataout_prefilter_en` in the SET13 register. In this way all the subsequent filters are bypassed.

6.3.3 High resolution low bandwidth signal path (HRLB)

Figure 5. HRLB digital signal path

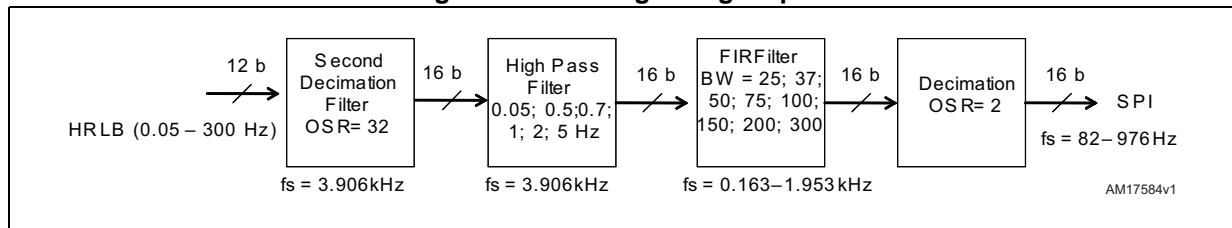

After the first decimation filter, a second decimation is performed in order to reduce the sampling frequency and, in the same time, to cut the high frequency signal part. The second decimation for HRLB signal is fixed to 32 and the output sampling frequency is 3.906 kHz. After that, a High Pass Filter is implemented. The -3 dB cut-off frequency is variable with 6 possible values: 0.05, 0.5, 0.7, 1, 2 and 5 Hz (`hc_dig_ecghpf_sel_r<0:2>`). After the HPF, a FIR filter with selectable bandwidth of 25, 37, 50, 75, 100, 150, 200 and 300 Hz (`hc_dig_ecglpf_sel_r < 0 : 2 >`) is implemented. At the end, a further decimation by 2 is inserted. Finally, the output signal is sent to the SPI block.

The following parameters can be set through the SPI interface:

- Low Pass Filter cut-off frequency: 25, 37.5, 50, 75, 100, 150, 200, 300, 600 Hz (`hc_dig_ecglpf_sel_r`);
- High Pass Filter cut-off frequency: 0.05, 0.5, 0.7, 1, 2, 5 Hz (`hc_dig_ecghpf_sel_r`);
- Cut-off start frequency of the high pass digital filter for the start-up procedure (`hc[1,2,3]_dig_hpf_sel_r`). Active only when recovery mode is OFF.

6.3.4 Low resolution high bandwidth signal path (LRHB)

The LRHB signal path takes the same signal of 12 bits 125 kHz, coming from the 1st decimation filter, as input. Linear phase response is an important parameter. This can only be achieved by using FIR filters. Implementing FIR filters to filter a 5 kHz with a sampling frequency of 125 kHz will require a lot of taps in the filter. As with the HRLB path low pass filter, a decimation step is performed to lower the sampling frequency so to decrease the required taps in the FIR filters.


The LRHB signal can be provided with different cut off frequencies for low and high pass filters. As shown in [Figure 6](#), the configuration of the digital blocks is changed in case of 5 kHz and 10 kHz low pass cut off frequencies.

A decimation step of 2 is done for the 10 kHz case and a decimation of 4 for the 5 kHz one, in this way the same FIR filter with only 4 taps is used in both cases. Implementing this decimation step with a good pass-band characteristic can be achieved with a CIC decimation filter.

For the 10 kHz low pass filter case, the FIR filter follows the first decimation filter, then a new decimation by 2 and finally the IIR high pass filter.

For the 5 kHz case, the FIR and IIR filters are swapped each other and, the decimation rate of the first filter is doubled.

Figure 6. LRHB signal path

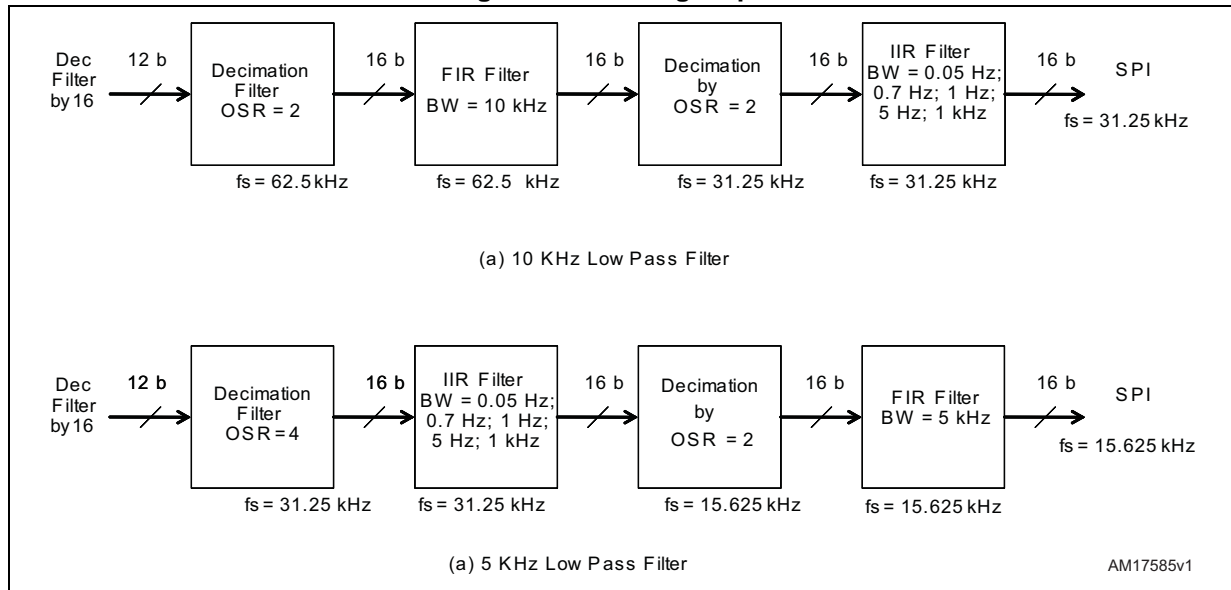

The following parameters can be set through the SPI interface:

- Low Pass Filter cut-off frequency: 5, 10 kHz (`hc_dig_pmlpf_sel_r`);
- High Pass Filter cut-off frequency: 0.05, 0.7, 1, 5, 1000 Hz (`hc_dig_pmhpf_sel_r`);
- Connection of the two LRHB signal paths to any of the three biopotential channels (`pm_sel_r`);

The LRHB signal path provides also a signal amplitude detection function. This function is useful as pacemaker detection (PMD) in ECG systems where reduced ODR, fewer MIPS for the host and low power consumption are key features. Integrated hardware detection of the pacemaker pulse allows the device to meet these requirements.


The 9 most significant bits without sign of the LRHB (16 bit) are compared with a user selectable threshold of 9 bit (`hc_pmd_thres_r`). When the threshold value is higher than the absolute value of the LRHB signal the output signal (PMD) is asserted high. Two PMD signals are available at DGIO1 and DGIO2 outputs. In ECG application these signals provide the pace maker detection signal. Since the comparison is done at digital level, the threshold value must be changed according to the gain setting.

For example, if a 0.2 mV value must be detected at the input of the channel and the threshold is set at 00000001, since one LSB of the ADC is 24 μ V, the 0.2 mV represents the 6th bit of the LRHB word with a gain of 8 or the 9th bit with a gain of 64. Since the comparison is done with the 9 MSBs, in the first case the PMD signal will be always low while in the second case the PMD will change in the same way as the 9th bit of the LRHB word.

6.4 Lead off detection

During ECG measurement and especially during a long period of monitoring, the electrode to skin contact check is needed in order to guarantee an adequate impedance value for a good signal acquisition. The HM301D provides two types of contact check: DC and AC

Figure 7. Contact check architecture

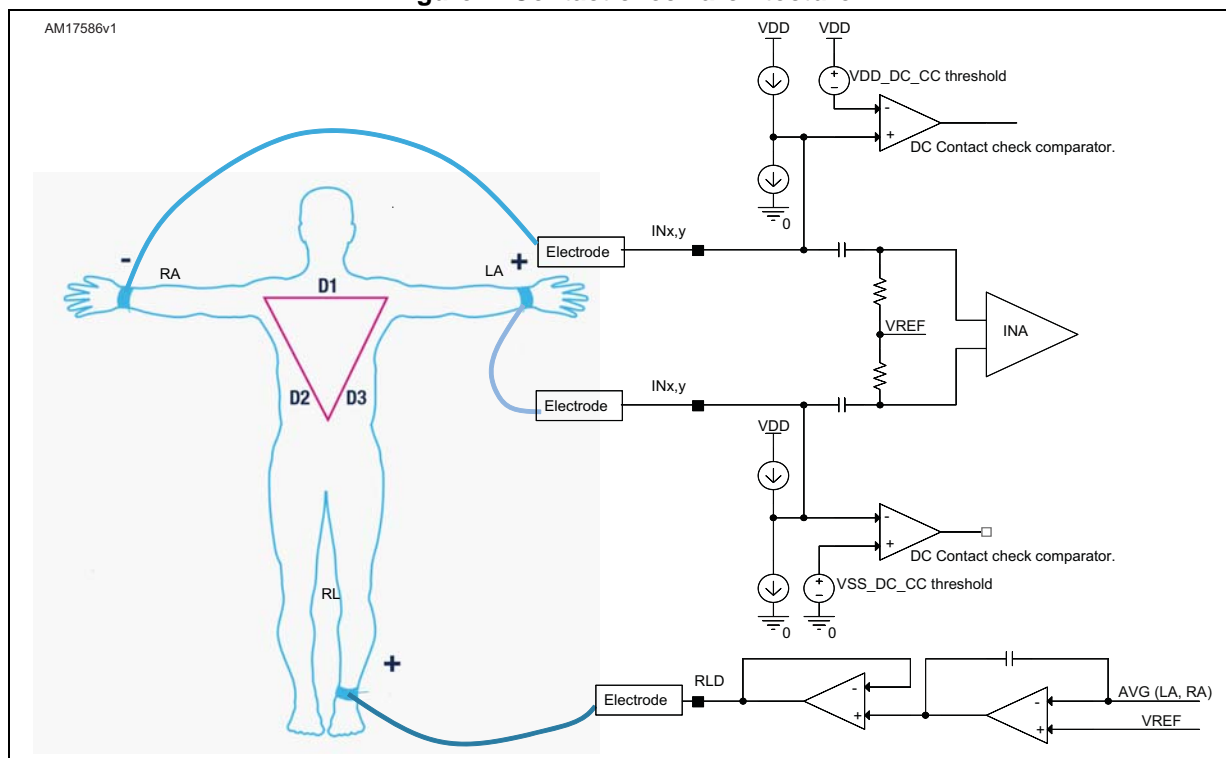

6.4.1 DC contact check

One current source and one current sink are connected at each of the 6 inputs of the biopotential channels. Two comparators are also connected at each pin. Each of the 6 current sources can be activated by setting the `in[1-3]_contact_pdp_r` bits while the 6 current sinkers are activated by setting the `in[1-3]_contact_pdn_r` bits. According to the electrode configuration, the proper current source/sink must be activated. A small selectable current (25, 50, 100, 200 nA) is injected by the current source through one electrode and body of the patient and back into the HM301D through another electrode where the right current sinker is turned on and having the same current value setting. This current generates a voltage drop that is detected by the comparators connected to each pin. The comparator threshold is also selectable in a different way for the high side comparators (`cck_threshp_sel_r`) and for the low side comparators (`cck_threshn_sel_r`). There are 16 possible comparator threshold values.

The maximum current mismatch between one current source and one current sinker is 10%, in this way the DC current going to the body is very small.

6.4.2 AC contact check

The AC contact check is based on the same principle of the DC contact check. In this case, an AC current (square wave) with a 2.5 kHz or 5 kHz (`hc_curinj_freq_r`) frequency is injected through the electrodes. The possible current values are 5, 10 or 20 μA . The quality of the electrode contact will be then evaluated by the host MCU by analyzing the injected frequency component in the LRHB signal.

For each biopotential channel the AC current source connected to the positive pin of the differential input is 180° out of phase with the one connected to the negative pin. In this way the current flows through the body and returns to the negative pin. When the contact

between two electrodes, each connected to the positive or negative inputs of two different channels, has to be checked, then it is necessary to reverse the phase of one of two involved AC current generator. The hc[1-3]_phaserev_r bits allow doing it so that any electrode configuration can be implemented.

The AC current generator is enabled by setting the relative hc[1-3]_curinj_en_r bit. In addition, by setting the hc_curinj_en_ext bit it is possible to enable/disable the AC current generators through an external logic signal applied to the DIGIO2 pin. This signal will be AND-ed with the hc[1-3]_curinj_en_r bits, so that only the enabled current generators will be turned on.


6.5 Impedance channel

The goal of the impedance channel is to measure the impedance of the body and to measure the variation of this impedance due to the respiration. In reality the measured impedance won't be the impedance of the body alone but the series connection of the body with the board protections, the 2 electrodes and with skin and gel impedances. These values must be taken into account when reading the impedance values of HM301D.

The impedance circuit detects impedance values by injecting a high frequency square wave AC current through the CIP and CIN pins and monitoring the resulting voltage (*Figure 8*).

High frequency is imposed both for safety reasons and due to the electrodes' band pass. To avoid electrode polarization the average injected current is minimized.

Figure 8. Impedance channel architecture

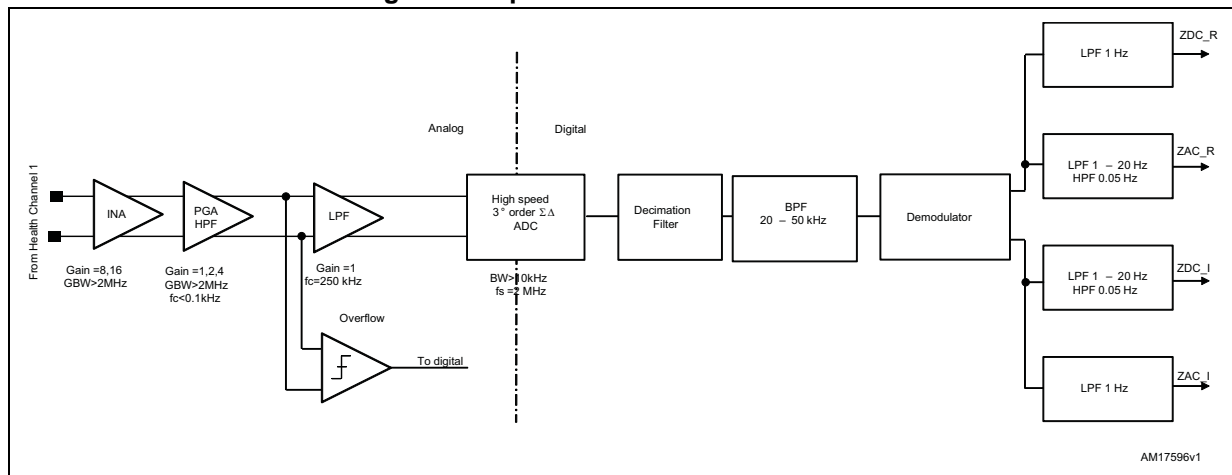

The body impedance is used as an indicator to determine biological parameters, such as those used for galvanic skin response evaluation and patient fluid status check. Furthermore, in automated external defibrillator (AED) applications, body impedance evaluation is needed in order to deliver the proper amount of energy to the patient. This function has been designed considering application-specific electrodes (i.e. with polarity).

The modulated impedance (AC impedance) measurement principle is based on bio-impedance measurement on the patient's thorax and allows the measurement of respiration concurrently with the ECG and pacemaker measurements using two standard ECG electrodes. The time variation of body impedance due to respiration and chest movement is measured. This allows breath rate evaluation and provides information about movement artifacts that can affect ECG measurement.

The impedance is measured by the injection of an AC current at 31.25 kHz and by measuring the resulting voltage across it. The current value can be chosen among three different values: 5, 10 and 20 μ A. Since this current is injected using different pins from the ones where the voltage is measured, a 4 wire measure (force and sense principle) is implemented.

Even if unpractical in real applications, using 4 different electrodes is really helpful to improve the accuracy of the impedance measurement. Anyhow using only 2 electrodes but separating the PCB path of force and sense until the cable connector, will bypass all the impedances of the application (protections, PCB tracks, etc) which usually have higher values than the ones that must be measured. For example, in ECG systems, the defibrillator and ESD protection resistors could be as high as 25 k Ω , while the measured body resistance is \sim 0.5 k Ω .

The impedance channel differential input is connected to the same input of biopotential channel 1 (see [Figure 1](#)).

The impedance channel outputs a real part and an imaginary part of the modulated impedance. This is obtained by IQ demodulation in the digital part of the channel which introduces additional gain and phase shift.

6.5.1 Analog section

All analog blocks of the impedance channel are the same as their counterparts of the biopotential channel except for the low pass filter which has now a cut-off frequency of 250 kHz.

Another difference is the ADC which is now a 3th order cascaded (2-1) low pass-delta-sigma. A second order converter plus an extra stage that converts the quantization noise are implemented. Therefore the ADC will have 3th order noise shaping.


The following parameters can be set through the SPI interface:

- Current injection frequency: 20, 25, 31, 35, 41, 45, 50 kHz (`imp_curinj_freq_r`);
- Current injection value: 5, 10 20 μ A (`imp_curinj_cur_r`);
- IA Gain: 8, 16 (`imp_ina_gain_r`);
- PGA Gain: 1,2, 4 (`imp_pga_gain_r`);

6.5.2 Digital section

[Figure 9](#) shows the 3rd order $\Sigma\Delta$ ADC followed by the filters in the impedance channel. The signal is first decimated and band pass filtered so to get sampling frequency of 4 times the signal frequency. An IQ-demodulator splits the signal in a real (I) and imaginary (Q) component. The result is again decimated before a final high pass filter at 0.05 Hz and low pass filter at 20 Hz or 1 Hz. The high pass filter is used to extract the ac component in combination with the 20 Hz or (after extra decimation) 1 Hz low pass filter. For the dc-component, only the 1 Hz low pass filter is used, without the high pass filter.

Figure 9. Impedance channel digital section

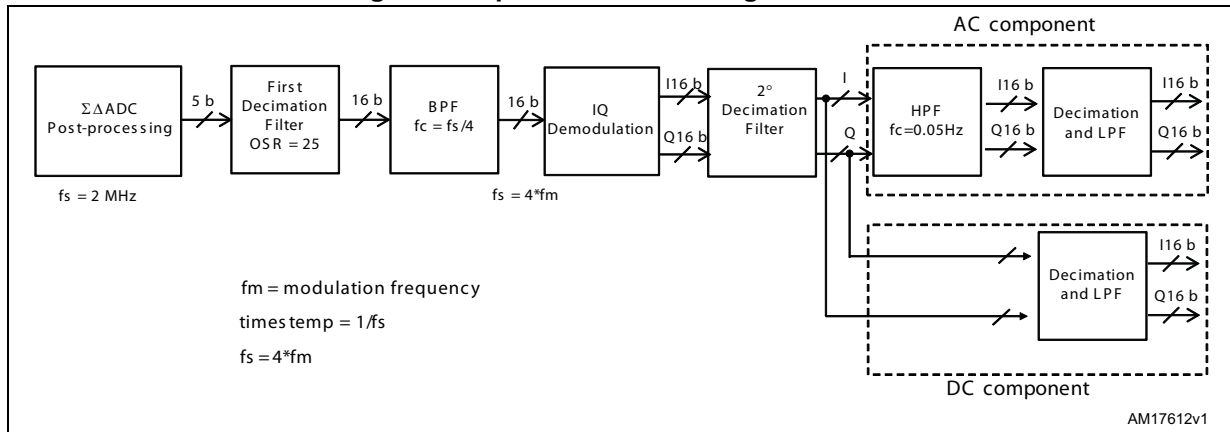

The following parameters can be set through the SPI interface:

- Digital Low Pass filter cut-off frequency: 1 or 20 Hz (imp_dif_lpf_sel_r)

6.6 Drivers

The global architecture for the drivers is shown in [Figure 10](#). The drivers operation is specifically designed for ECG systems. In particular the WCT (Wilson common terminal) is used in unipolar ECG systems, while RLD is the right leg driver for ECG which allows reducing system disturbances. The Shield driver is used in case of shielded cable.

An important role is played by the four AVG buffers. The positive inputs of these buffers are connected to any of the INxy pins by programming the input connection matrix (inputcon_avg[1-4]_r). In this way, the average value of any combination of the biopotential channels can be created. The output of the AVG buffers is fed to the shield driver and RLD driver. Each of the four AVG buffers can be turned on/off by setting the avg_en_buf[1-4]_r bit. It is important to turn on only the AVG buffers used because the summing resistors will be programmed according to the numbers of AVG buffers which are on.

In addition the right number of AVG buffers used must be written in the avg_numb_buf_r bits. This number will represent the total number of AVG buffers used also in the case of multiple connections of HM301D chips, where all the AVGIO pins are tied together.


The topology of the drivers is based on the following considerations:

It should not load the input signal. Therefore the electrode inputs are buffered with unity gain buffers.

The unipolar measurements should have similar accuracy as the bipolar measurements. This basically means that the total noise contribution of the 3 unity gain buffers must be smaller than the total noise contribution of the entire biopotential channel.

The bandwidth of the WCT circuit must be enough to not generate too much delay.

Figure 10. AVG buffers

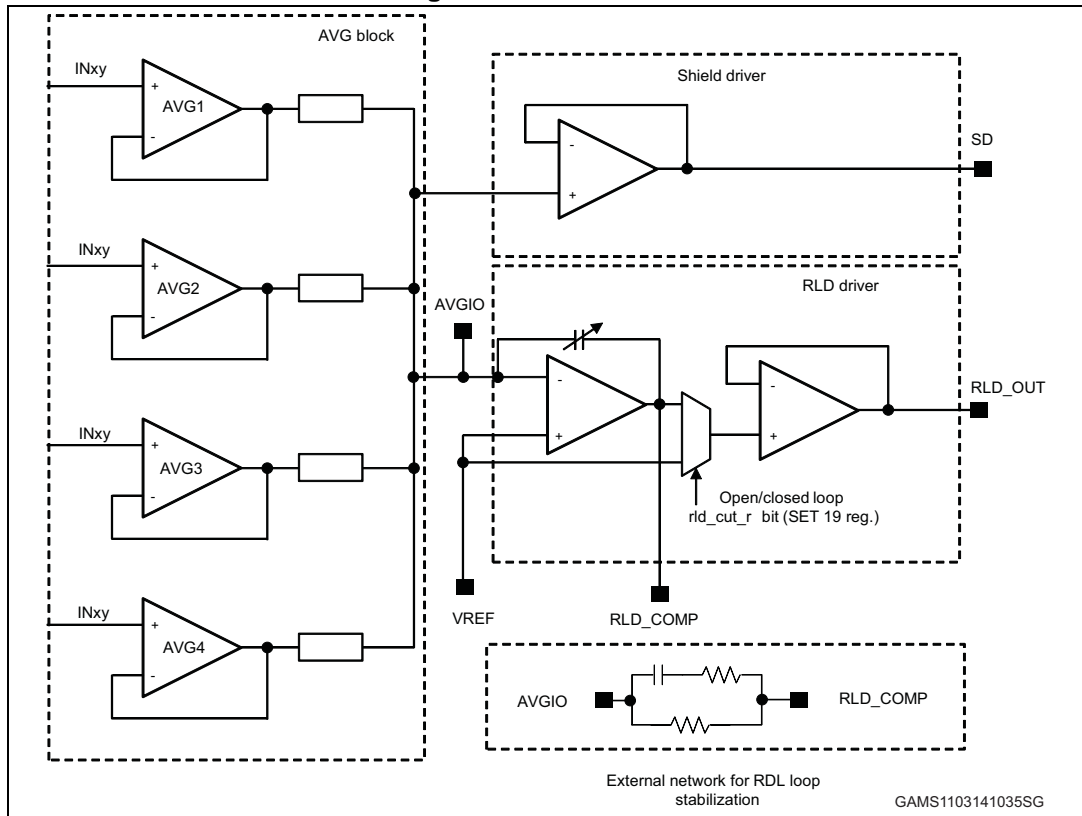

6.6.1 Right leg driver

The human common mode must be driven in order to set it at the HM301D reference. The driver is connected to the right leg of the patient by means of an electrode, and the effect of the RLD is to reduce the effective electrode impedance. When the ICs are chain-connected only the RLD of one chip will be connected to the electrode, because the total average is already performed by the AVG buffers. Applications without the right leg electrode are considered and, in these cases, RLD can be used to drive the electrode signals by means of 2 external resistors.

The RLD_COMP pin allows the connection of an external compensation network in case of need for the RLD loop stabilization.

6.6.2 Shield driver

If shielded electrode wires are used, the shield must be driven in order to reject interference from the main. The shield is driven to the average value of all the electrode signals (also considering multi chip configuration).

6.6.3 Wilson common terminal (WCT)


WCT is the standard potential used to evaluate precordial leads in ECG applications. This potential is defined and evaluated as the average of right arm, left arm and left leg electrode potentials. This value is available on a dedicated pin as an analog signal.

The WCT buffer needs to be fast enough to have a low delay. The bandwidth of the WCT driver is 0.5 MHz at least, but since the WCT output goes off-chip, it has to steer the input of

the biopotential channels and the load of the PCB connections. The average is made with 3 times 100 kΩ resistors.

The positive inputs of the 3 WCT buffers are tied to inputs of the first three AVG buffers (AVG1,2,3). So the inputcon_avg[1-3]_r bits determine where the three inputs of the WCT buffers are connected.

Figure 11. WCT buffer

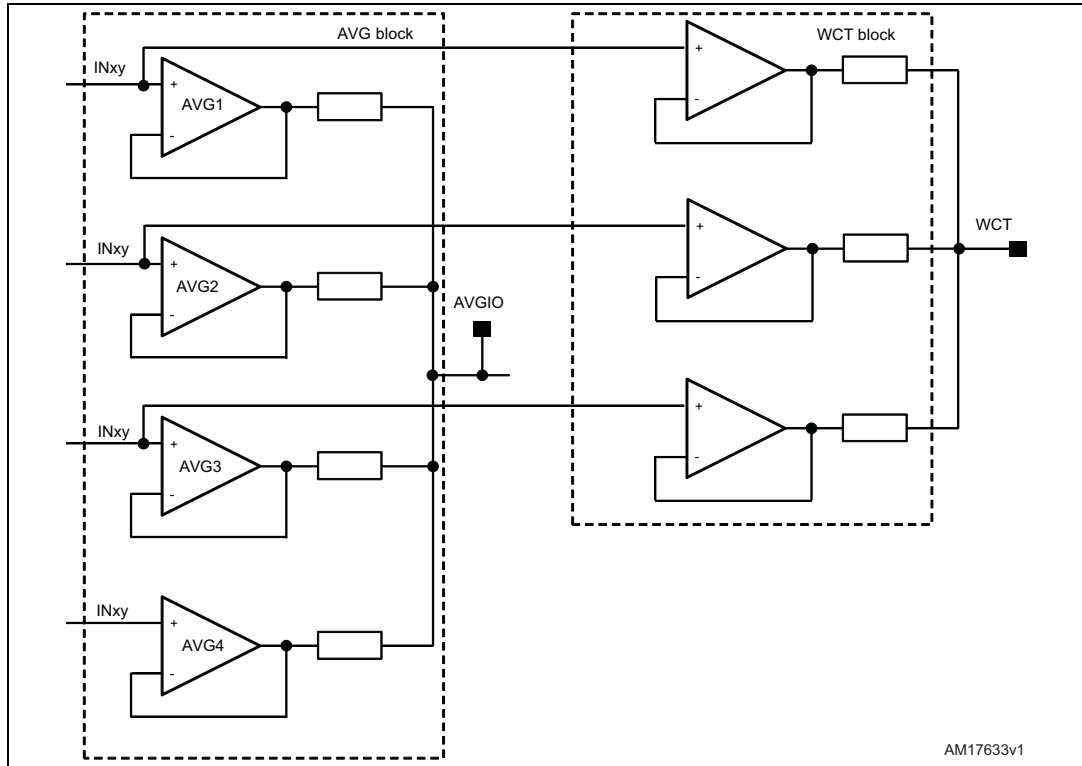

6.7 TM and RST pin configuration

The HM301D RST pin can be configured as input and output by the TM pins. When TM0 and TM1 pins are both grounded, the RST pin is configured as an output and the RST pin outputs a POR signal.

If TM1 is grounded and TM0 is connected to DVDD the RST pin is configured as an ENABLE input. When pulled high, all on chip circuitry is powered up when asserted low the device goes in sleep.

Table 10. Functional modes

TM1	TM0	RST pin	Function	Description
DVSS	DVSS	POR	Digital Output	The RST pin outputs POR: <ul style="list-style-type: none"> · High → device off · Low → device on
DVSS	DVDD	EN	Digital Input	The RST pin is configured as Enable: <ul style="list-style-type: none"> · High → power up · Low → power down
DVDD	DVSS	RES	-	Reserved
DVDD	DVDD	RES	-	Reserved

6.8 Digital machine

The digital part of the HM301D performs the preprocessing and filtering of all the digital signals coming from 4 analog channels. This part has been already described in the biopotential and impedance channel sections. In addition it manages all the device operation related to operating modes, trimming and test procedures, start-up sequence. The digital part can be configured through SPI and has a non-volatile memory which carries the trimming words for the analog building blocks. In HM301D the data can be retrieved by two methods: packets streaming mode and read data command mode. These two procedures can be selected by meas_mode bit (SET22 <7>).

6.8.1 Operating modes

The HM301D has the following operating states: sleep, boot, standby, ready, measure, recovery.

6.8.2 Sleep

This state is active when in any other state the RST pin is asserted low

6.8.3 Boot

This state is reached 100 μ s after the RST pin is gone to V_{DD} . This function is implemented with an internal counter so to wait the right time for the analog blocks to be stable. The device stays in this state for 600 μ s before automatically moving to standby.

6.8.4 Standby

- Packets streaming mode (meas_mode = 0).

This state is reachable in two ways:

- From Boot state. This means that the boot is correctly performed;
 - From Measure state, by pulling up the CS pin. This means that the user asks to exit from the Measure mode in order to load through SPI a new configuration (see SPI communication for details).
- Read data command mode (meas_mode = 1)

This state is reachable in two ways

- From Boot state. This means that the boot is correctly performed
- From Measure state putting the settings_ok_r bit to zero


6.8.5 Ready

This state is reached from Standby mode when the bit settings_ok_r (3Dh) is set to 1 and the clock is working correctly. This means that the user has loaded all the configurations and the clock is running correctly. This state is not present when meas_mode = 1.

6.8.6 Measure


- Packets streaming mode (meas_mode = 0).
 - This state is reachable from the in ready state putting the CS pin low. When entering the measure state the device automatically initiates a first fast recovery procedure end then outputs the data on SPI
 - When in measure state the device can pass to stand-by state by pulling the CS pin high.
- Read data command mode (meas_mode = 1)
 - This state is reachable from standby state putting the settings_ok_r bit to 1. When entering the measure state the device automatically initiates a first fast recovery procedure.
 - When in Measure state the device can pass to stand-by state setting the settings_ok_r bit to 1.

Figure 12. State machine for packets streaming mode (meas_mode = 0)

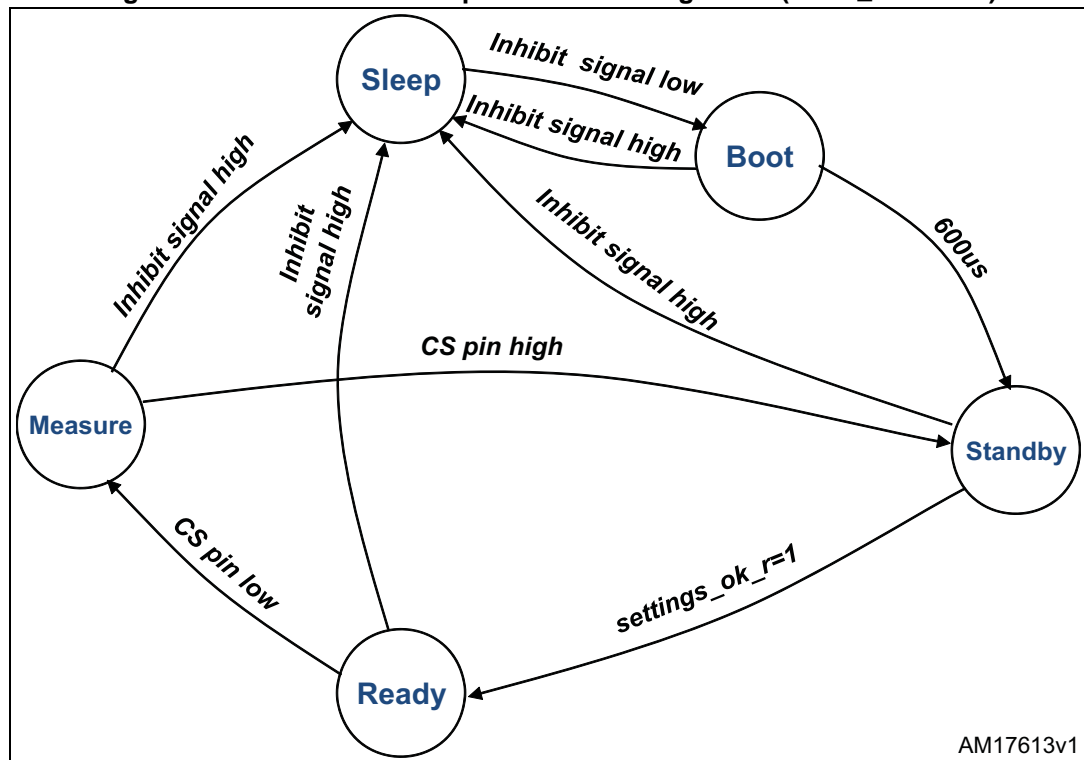

AM17613v1

Figure 13. State machine for packets streaming mode (meas_mode = 1)

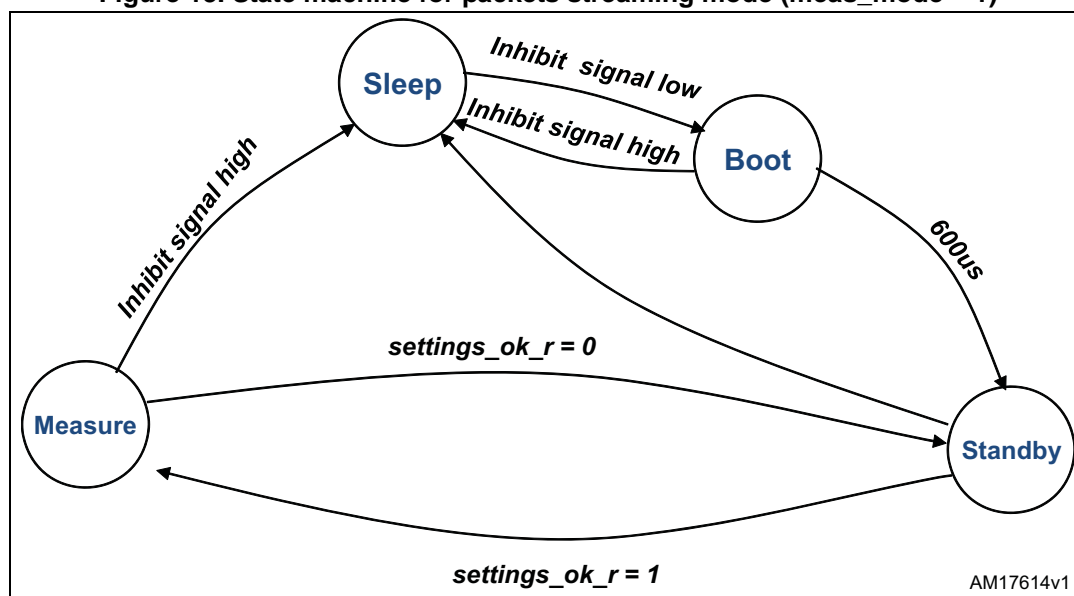

6.8.7 Fast recovery

During an overvoltage, overflow condition or at start-up, i.e. a condition where the input voltage is too large or zero, the digital state machine initiates the recovery mode.

This procedure is activated when entering the Measure state and when an overflow condition lasts for a longer time than a programmed blanking time. This time is programmable from 2.5 ms to 37.5 ms in 2.5 ms steps by setting the `recovery_time_r` bits.

The recovery procedure can be disabled by setting `recovery_time_r = 1111`. In this condition, the digital high pass filters are set by the `hcX_dig_hpf_sel_r` (registers 38h and 39h) and not by the `hc_dig_ecghpf_sel_r` and `hc_dig_pmhpf_sel_r`. With the recovery mode disabled, it is possible to change the cut-off frequency of the analog high pass filters by changing the `hc[1-3]_rhp_sel_r` bits.

At the beginning of the Recovery mode, the HP filters of all the channels, both in the digital as well as in the analog domain, are switched to their highest (5 Hz) cut-off frequency, then they are switched to lower frequencies. From 5 Hz the cut-off is changed to 0.7 Hz and then to 0.05 Hz. The timing between two different cut-off frequencies is programmable between 0 and 1 s with 200 ms steps (`filter_swichtime1_r` / `filter_swichtime2_r`). So when the maximum time is chosen, the total recovery time is 2 s: 1s for the switching time from 5 Hz to 0.7 Hz and 1s for the switching time from 0.7 Hz to 0.05 Hz.

The digital HP filter is switched in the same way as the analog HP filter. The only difference is that it stops at the frequency which is selected by the `hc_dig_ecghpf_sel_r` and `hc_dig_pmhpf_sel_r` bits. For instance, if the user selects a HP cut-off of 0.7 Hz then the filter stops at 0.7 Hz. When it is 1 Hz the filter switches to 1 Hz instead of 0.7 Hz.

During recovery mode all the AC current injection blocks are disabled, so the signals, `hcX_curinj_en` and `imp_curinj_en` are set to 0.

6.9 GPIO configuration

The HM301D has 3 digital GPIOs. DGIO0 and DGIO1 are always used as outputs while DGIO2 can be configured as input or output by changing the `dgio2_config_r` bit (address 40h bit #2).

Each DGIO has his own multiplexer that can be configured by changing the corresponding `digiox_mus_sel_r<3:0>` (registers SET25 and SET26). The multiplexer configuration is shown in the following tables.

Table 11. Digital GPIO output signals (DGIO0)

Register SET 26 - address 46 hex - <7:4> DGIO0_muxsel_r <3:0>	DGIO0
0000	pm_rsh
0001	clk_o
0010	pmd1
0011	pmd2
0100	imp_adc_pdm1_o
0101	fchop_o
0110	por_o
0111	not used
1000	ecg_rsh
1001	z_rsh
1010	prefilt_rsh
1011	in_contact_out_flag1
1100	in_contact_out_flag4
1101	in_cck_out1
1110	in_cck_out4
1111	hc1_overflow_flag

Table 12. Digital GPIO output signals (DGIO1)

Register SET 25 - address 45 hex - <3:0> DGIO1_muxsel_r <3:0>	DGIO1
0000	pmd1
0001	hc1_adc_pdm_o
0010	hc2_adc_pdm_o
0011	hc3_adc_pdm_o
0100	imp_adc_pdm2_o
0101	psmon0
0110	not used
0111	ecg_rsh
1000	z_rsh
1001	prefilt_rsh
1010	pm_rsh
1011	in_contact_out_flag2
1100	in_contact_out_flag5
1101	in_cck_out2
1110	in_cck_out5
1111	hc2_overflow_flag

Table 13. Digital GPIO output signals (DGIO2)

Register SET 25 - address 45 hex - <7:4> DGIO2_muxsel_r <3:0>	DGIO2 (dgio2_config_r=1)
0000	pmd2
0001	hc1_overflow_o
0010	hc2_overflow_o
0011	hc3_overflow_o
0100	imp_overflow_o
0101	psmon1
0110	not used
0111	z_rsh
1000	pm_rsh
1001	imp_overflow_flag
1010	ecg_rsh
1011	in_contact_out_flag3
1100	in_contact_out_flag6
1101	in_cck_out3
1110	in_cck_out6
1111	hc3_overflow_flag

Description of the signals:

- pm_rsh:
 - This signal provides the information about a new data refresh of the LRHB signal path inside the HM301D. This signal must be used to synchronize the MCU readings. In this case the data must be retrieved using the data packet streaming procedure (Meas_mode=0). As soon this signal goes high, the MCU can send a train of 80 clock pulses in order to read 64 bits of the data stream.
- ecg_rsh:
 - This signal provides the information about a new data refresh of the HRLB signal path inside the HM301D. This signal must be used to synchronize the MCU readings. In this case the data must be retrieved using the normal SPI data reading procedure. As soon this signal goes high, the MCU must read directly the ECG_OUT registers using the word reading procedure as described in [Figure 15](#). To enable the SPI data reading the Meas_mode bit in SET 22 register must be set to 1.
- z_rsh:
 - This signal provides the information about a new data refresh of the impedance channel path inside the HM301D. This signal must be used as trigger to synchronize the MCU readings. In this case the data must be retrieved using the normal SPI data reading procedure. As soon this signal goes high, the MCU must read directly the Impedance registers using the word reading procedure as described in [Figure 15](#). To enable the SPI data reading the Meas_mode bit in SET 22 register must be set to 1

- `prefilt_rsh`:
 - This signal provides the information about a new data refresh of the pre-filtered signals. This signal must be used to synchronize the MCU readings. In this case the data must be retrieved using the data packet streaming procedure. As soon this signal goes high, the MCU can send a train of 48 clock pulses in order to read 64 bits of the pre-filtered data stream.
- `pmd1`, `pmd2`:
 - These signals represent the output of the signal amplitude detection of the LRHB signal path of the biopotential channels. `pmd1` and `pmd2` can be configured to provide the data of CH1, CH2 and CH3 according to the `pm_sel_r` bits (address `28h<6:4>`).
- `hc1_adc_pdm_o`, `hc2_adc_pdm_o`, `hc3_adc_pdm_o`:
 - 1bit 2Mhz output streams of the ADCs of the three acquisition channels;
- `hc1_overflow_o`, `hc2_overflow_o`, `hc3_overflow_o`, `imp_overflow_o`:
 - Overflow signals of the three acquisition channels and impedance channel;
- `in_contact_out_flag1`, `in_contact_out_flag2`, `in_contact_out_flag3`, `in_contact_out_flag4`, `in_contact_out_flag5`, `in_contact_out_flag6`: contact check flags go high if the comparator threshold is crossed. The status of this flags is latched out at the rising edge of internal generated clock.
- `in_contact_out1`, `in_contact_out2`, `in_contact_out3`, `in_contact_out4`, `in_contact_out5`, `in_contact_out6`: outputs of the contact check comparator. These signals are the outputs of the contact check comparator and give the same information of the `in_contact_out_flagx` but in asynchronous way.
- `hc1_overflow_flag`, `hc2_overflow_flag`, `hc3_overflow_flag`, `imp_overflow_flag`:
 - HRLB channels and impedance channel overflow flags
- `imp_adc_pdm1_o`:
 - First bit of the $\Sigma\Delta$ stream of the ADC of the impedance channel;
- `imp_adc_pdm2_o`:
 - Second bit of the $\Sigma\Delta$ stream of the ADC of the impedance channel;
- `fchop_o`:
 - Chopping signal for the input amplifiers and signal for AC contact check current injection;
- `clk_o`:
 - oscillator output;
- `Por_o`
 - Power on reset signal.
- `psmon0`, `psmon1`
 - power supply voltage monitor (see [Figure 6.11](#)).

The DGIOx can be also configured as an input.

- To configure DGIO0 as input set `dgio0_config_r` bit=0 (SET23 DIGIO_IO address 40h bit #0).
- To configure DGIO1 as input set `dgio1_config_r` bit=0 (SET23 DIGIO_IO address 40h bit #1).
- To configure DGIO2 as input set `dgio2_config_r` bit=0 (SET23 DIGIO_IO address 40h bit #2).

Following two tables give an overview of the digital input and output mux configuration

Table 14. Digital GPIO input signals

digioX_mux_sel[3:0]	DIGIO0	DIGIO1	DIGIO2
0000		impinj_ondem_en_i	accc_ondem_en_i

- impinj_ondem_en_i: when low, it disables impedance current injection;
- accc_ondem_en_i: when low, it disables AC contact check current injection

By connecting these pins to an MCU IO it is possible to turn on/off the ac current injection and impedance without interrupting the data stream of the SPI port.

6.10 SPI interface

The HM301D SPI port works as a bus slave. The SPI allows writing and reading the registers of the device.

The Serial Interface works with 4 wires: CS, SPC, SDI and SDO.

When in measurement mode the SPI port works in a particular way where no address is needed for reading the data but the device automatically send out the data in a particular output format, see [Section 6.13](#) for details.

The HM301D SPI is capable of being connected in a daisy chain when multiple chips are connected together (see [Section 6.10.3](#)).

CS is the serial port enable and it is controlled by the SPI master. It goes low at the start of the transmission and goes back high at the end. SPC is the serial port clock and it is controlled by the SPI master. It is stopped when CS is high (no transmission). SDI and SDO are respectively the serial port data input and output. Those lines are driven at the falling edge of SPC and should be captured at the rising edge of SPC. All the pins are idle when high.

6.10.1 SPI read

The read operation is performed by 32 clock pulses. In the first 16 pulses the master sends the read command byte and a dummy byte (FFh) through SDI pin with CS pin low. After that, the master must put the CS pin high and send the second 16 clock pulses in order to output the read command byte and the data byte through the SDO pin. The read command byte contains the READ/WRITE bit (MSB) and the register address.

Figure 14. Single byte reading


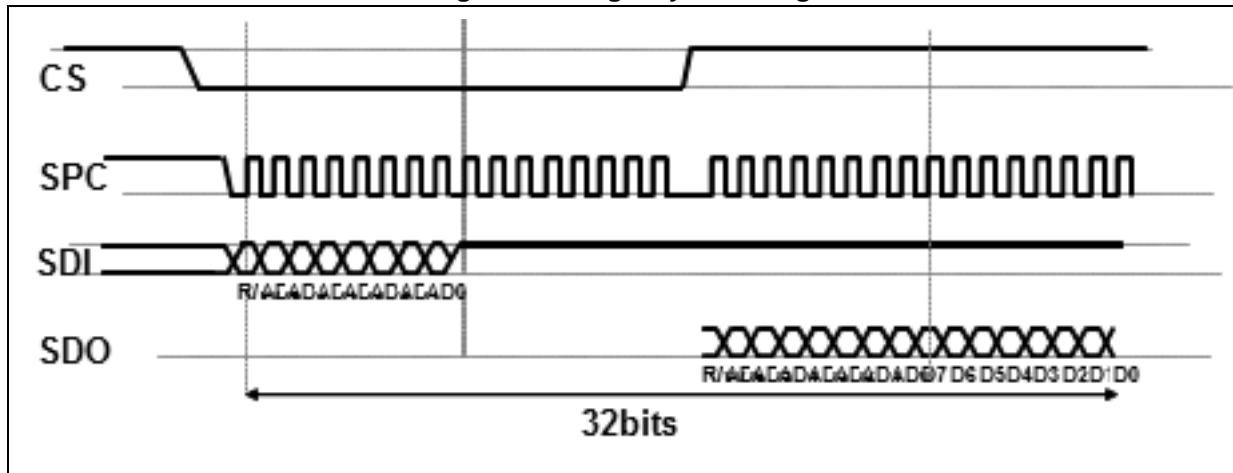


Table 15. Read command bytes

WRITE bit (MSB)	Register address						
1	AD6	AD5	AD4	AD3	AD2	AD1	AD0

The [Figure 15](#) shows the procedure for a double byte reading.

Figure 15. Double byte reading

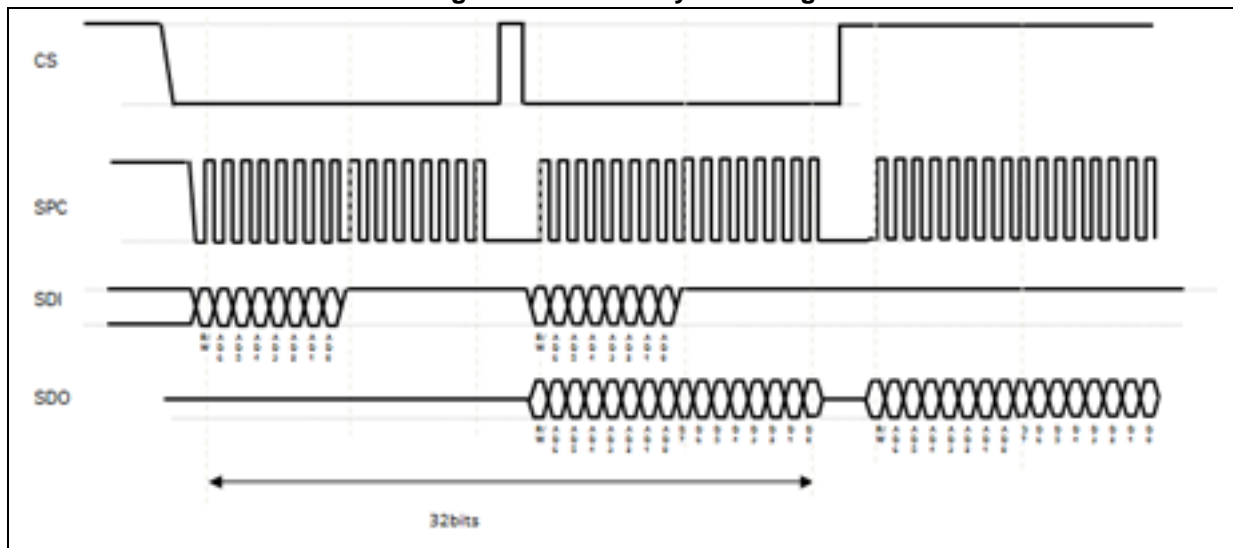

6.10.2 SPI write

The SPI Write command is performed with 16 clock pulses. In the first 8th bit the master sends the READ/WRITE command byte; in the second 8th bit the master sends the data byte to write. The command byte contains the READ/WRITE bit (MSB) and the register address (AD(6:0)). Both command byte and data byte must be written in MSB-first format.

Figure 16. Single byte writing

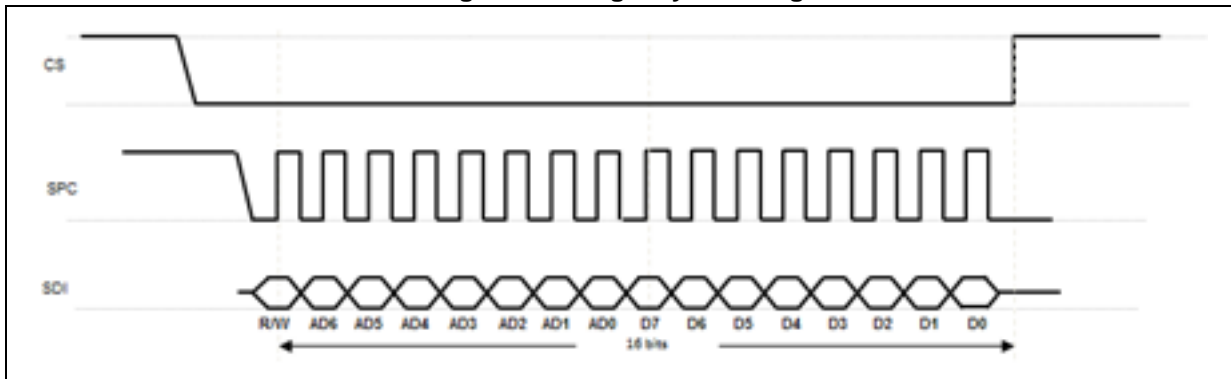



Table 16. Write command byte

WRITE bit (MSB)	Register address						
0	AD6	AD5	AD4	AD3	AD2	AD1	AD0

6.10.3 Daisy chain SPI

In the daisy chain SPI configuration, the first slave input (SDI) is connected to the MOSI and the first slave output (SDO) is connected to the second slave input (SDI) and so on. The last slave output is connected to the MISO of the master.


Figure 17. Example of daisy chain SPI connection with 3 HM301D

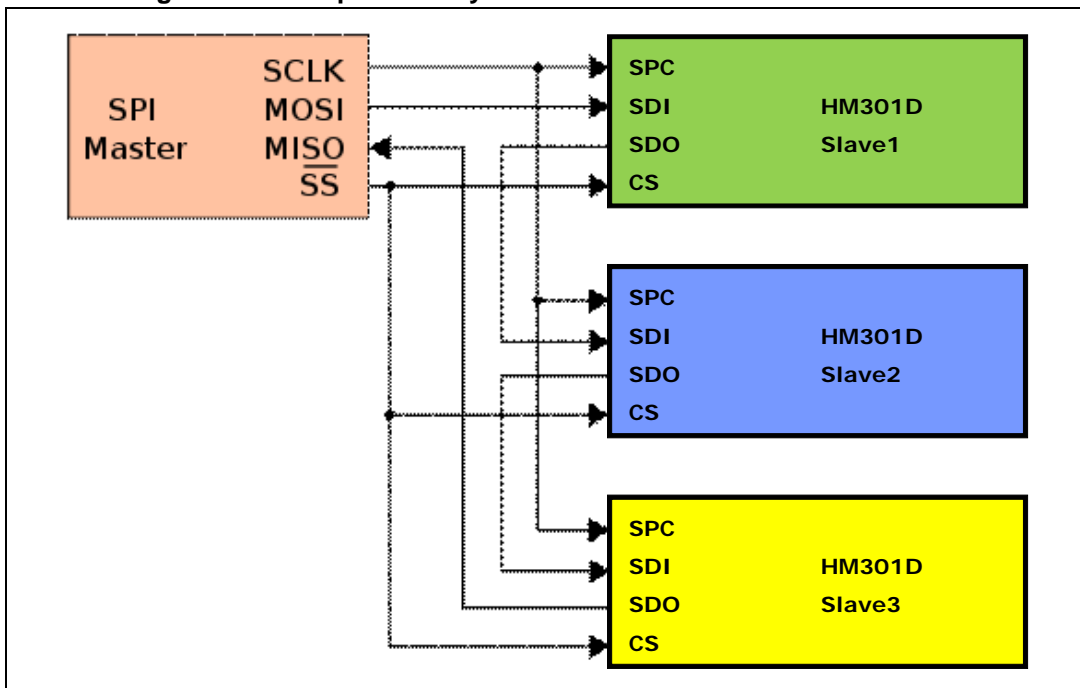

During the period in which CS stays high, the SPI port of each slave is designed to send out during the second group of clock pulses an exact copy of what it received during the first group of clock pulses. So all the SPI ports work as shift registers. When CS is low, all the slaves execute the commands at their respective SDI inputs.

Writing one register needs 16 pulses clock for each device connected in daisy chain. In the below example, three devices are connected in daisy chain so 48 clock pulses are needed to write a register into each of them. During the first 32 cycles the commands are shifted through the chain. In the last 16 bits, CS is pulled low and the devices execute the commands. In this way, each slave can receive its own command. It is also possible to send commands to just the first or the first two slaves by stopping the clock pulses at 16 or 32 respectively and, of course, pulling CS low accordingly.

Figure 18. Example of daisy chain SPI writing

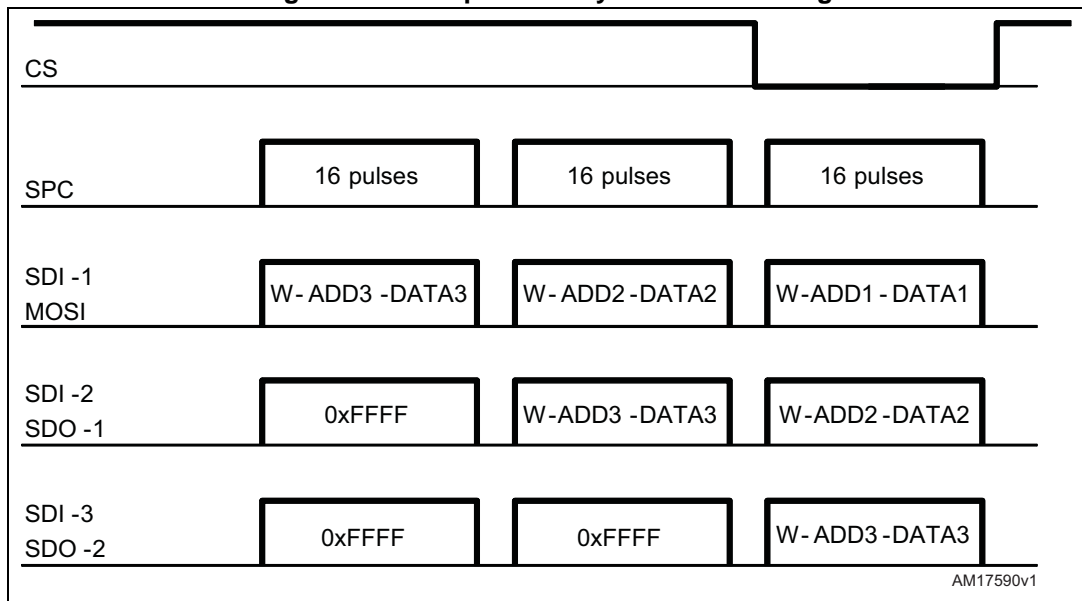


1. W: write bit
2. ADDx<0:6>: register address of the x device of the chain
3. DATAx<0:7>: data value to be written in the x device of the chain

Reading in daisy chain needs additional 16 cycles for each device. This is because the devices need the clock to shift the output data through the chain until the data coming from the first slave reaches the master input (MISO).

The picture below show an example of reading one register (different for each device) with three HM301D connected in chain.

Figure 19. Example of daisy chain SPI reading

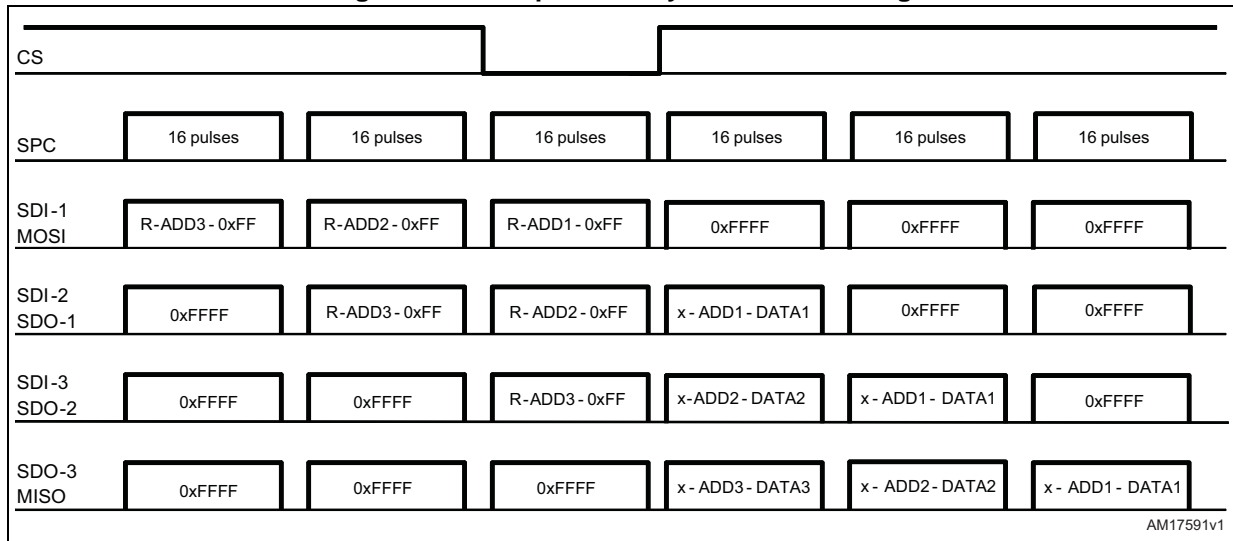

1. R: read bit
2. ADDx<0:6>: register address of the x device of the chain
3. DATAx<0:7>: data value read in the x device of the chain


See 0 for details about reading daisy chain SPI when HM301D is in measurement mode.

6.10.4 SPI timing

Table 17. SPI slave timings (IOVDD = 1.8 V)

Symbol	Parameter	Test condition	Min.	Max.	Unit
$t_c(SPC)$	SPI clock cycle		100		ns
$f_c(SPC)$	SPI clock frequency			10	MHz
$t_{su}(CS)$	CS setup time		6		ns
$t_h(CS)$	CS hold time		8		
$t_{su}(SI)$	SDI input setup time		5		
$t_h(SI)$	SDI input hold time		15		
$t_v(SO)$	SDO valid output time			50	
$t_h(SO)$	SDO output hold time		9		
$t_{dis}(SO)$	SDO output disable time			50	

Figure 20. SPI timing

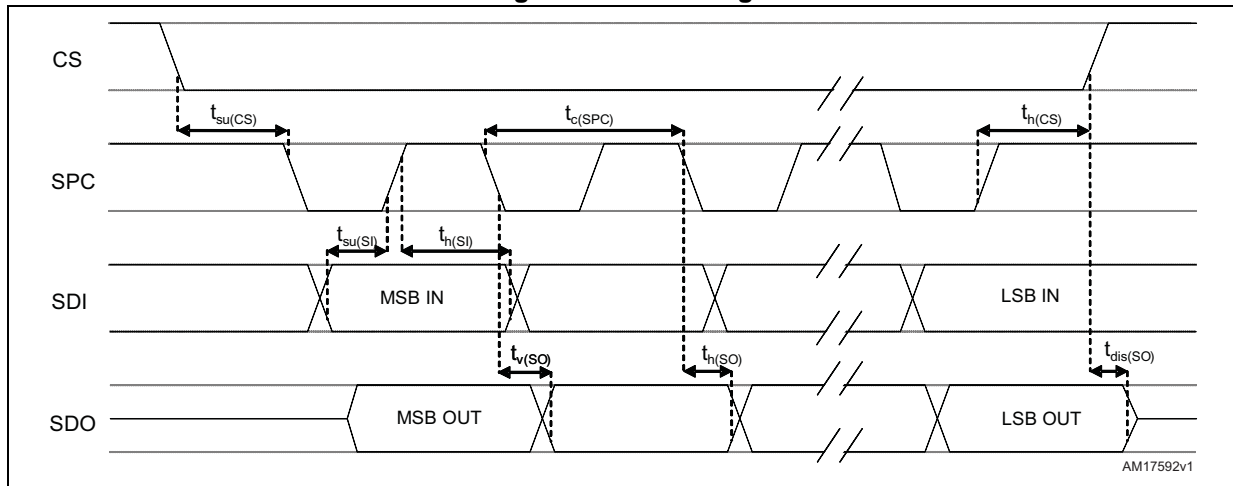

4. Values are guaranteed at 10 MHz clock frequency for SPI with 4 wires, based on characterization results, not tested in production.
5. Measurement points are done at 0.2 IOVDD and 0.8 IOVDD, for both input and output port.

6.11 Power supply voltage monitor

The HM301D is able to monitor the level of analog supply voltage and to give a 2 bits signal named psmon_out. The table below shows the meaning of the psmon_out<1:0>.

Table 18. Psmon_out signal

psmon_out_i<1:0>	Supply level
00	AVDD < 1.62 V
01	1.62 V < AVDD < 2.13 V
10	2.13 V < AVDD < 3.6 V
11	AVDD > 3.6 V

The psmon_out signal is available for SPI reading in the OUT_FLAG1 register (48h) or in the DIGIO1 and DGIO2 with proper configuration of DGIO multiplexer.

6.12 Registers MAP

Table 19. Registers MAP

Register name	Register description	Sub address	Type
SET0	Enable bits	27h	R/W
SET1	Active Pacemaker channels, current injection enables	28h	R/W
SET2	AVG Buffers	29h	R/W
SET3	Multi chip configuration, input matrix configuration	2Ah	R/W
SET4	input matrix configuration	2Bh	R/W
SET5	input matrix configuration	2Ch	R/W
SET6	input matrix configuration	2Dh	R/W
SET7	input matrix configuration	2Eh	R/W
SET8	Clock configuration, RLD connection	2Fh	R/W
SET9	DC contact check settings	30h	R/W
SET10	DC contact check settings	31h	R/W
SET11	DC contact check settings	32h	R/W
SET12	DC contact check comparators settings	33h	R/W
SET13	Gain of biopotential channels, AC contact check current injection	34h	R/W
SET14	Impedance channel settings	35h	R/W
SET15	Gain of impedance channel, LPF and HPF settings of LBHR path	36h	R/W

Table 19. Registers MAP (continued)

Register name	Register description	Sub address	Type
SET16	LPF and HPF settings of HBLR path	37h	R/W
SET17	Fast startup settings of analog and digital HP filter	38h	R/W
SET18		39h	R/W
SET19	AC current injection phase, RLD settings, LPF of impedance channel	3Ah	R/W
SET20	Recovery time settings, PM detection threshold	3Bh	R/W
SET21	PM detection threshold	3Ch	R/W
SET22	Start output data, HP filter switching time at start-up	3Dh	R/W
SET23	DIGIO2 input or output configuration	40h	R/W
SET24	Enable psmon, chop, current injection	44h	R/W
SET25	Multiplexer configuration for Digital GPIOs DIGIO1 and DIGIO2	45h	R/W
SET26	Multiplexer configuration for Digital GPIO DIGIO0	46h	R/W
Output Flags (READ ONLY)			
OUT_FLAG0	Overflow flags	47h	R
OUT_FLAG1	DC contact check flags	48h	R

Table 20. Registers MAP

Register name	Register description	Sub address	Type
ECG1_DATAOUT_1		49h	R
ECG1_DATAOUT_0		4Ah	R
ECG2_DATAOUT_1		4Bh	R
ECG2_DATAOUT_0		4Ch	R
ECG3_DATAOUT_1		4Dh	R
ECG3_DATAOUT_0		4Eh	R
ECG12_DATAOUT_1		4Fh	R
ECG12_DATAOUT_0		50h	R
ECG23_DATAOUT_1		51h	R
ECG23_DATAOUT_0		52h	R
ECG31_DATAOUT_1		53h	R
ECG31_DATAOUT_0		54h	R
PM1_DATAOUT_1		55h	R
PM1_DATAOUT_0		56h	R
PM2_DATAOUT_1		57h	R
PM2_DATAOUT_0		58h	R
IMPEDANCE_PHASE_AC_DATAOUT_1		59h	R
IMPEDANCE_PHASE_AC_DATAOUT_0		5Ah	R
IMPEDANCE_SQUARING_AC_DATAOUT_1		5Bh	R
IMPEDANCE_SQUARING_AC_DATAOUT_0		5Ch	R
IMPEDANCE_PHASE_DC_DATAOUT_1		5Dh	R
IMPEDANCE_PHASE_DC_DATAOUT_0		5Eh	R
IMPEDANCE_SQUARING_DC_DATAOUT_1		5Fh	R
IMPEDANCE_SQUARING_DC_DATAOUT_0		60h	R
CONTACT_CHECK_DATAOUT_1		61h	R
CONTACT_CHECK_DATAOUT_0		62h	R

Table 21. Data registers (readable only if meas_mode bit is 1)

Register name	Register description	Sub address	Type
ECG1_DATAOUT_1		49h	R
ECG1_DATAOUT_0		4Ah	R
ECG2_DATAOUT_1		4Bh	R
ECG2_DATAOUT_0		4Ch	R
ECG3_DATAOUT_1		4Dh	R
ECG3_DATAOUT_0		4Eh	R
ECG12_DATAOUT_1		4Fh	R
ECG12_DATAOUT_0		50h	R
ECG23_DATAOUT_1		51h	R
ECG23_DATAOUT_0		52h	R
ECG31_DATAOUT_1		53h	R
ECG31_DATAOUT_0		54h	R
PM1_DATAOUT_1		55h	R
PM1_DATAOUT_0		56h	R
PM2_DATAOUT_1		57h	R
PM2_DATAOUT_0		58h	R
IMPEDANCE_PHASE_AC_DATAOUT_1		59h	R
IMPEDANCE_PHASE_AC_DATAOUT_0		5Ah	R
IMPEDANCE_SQUARING_AC_DATAOUT_1		5Bh	R
IMPEDANCE_SQUARING_AC_DATAOUT_0		5Ch	R
IMPEDANCE_PHASE_DC_DATAOUT_1		5Dh	R
IMPEDANCE_PHASE_DC_DATAOUT_0		5Eh	R
IMPEDANCE_SQUARING_DC_DATAOUT_1		5Fh	R
IMPEDANCE_SQUARING_DC_DATAOUT_0		60h	R
CONTACT_CHECK_DATAOUT_1		61h	R
CONTACT_CHECK_DATAOUT_0		62h	R

6.12.1 Application settings (Read/Write)

Table 22. SET0 CH_ENABLE (ADDR 27h)

BIT	Name	Default	Description
7	sd_en_r	0	Enable Shield driver
6	wct_en_r	0	Enable ALL WCT buffers
5	dig_en_r	0	Enable digital filtering of ALL health channels
4	d2se_en_r	0	Enable diff2se buffer of ALL health channels
3	imp_en_r	0	Enable Impedance Channel
2	hc3_en_r	0	Enable Health Channel 3
1	hc2_en_r	0	Enable Health Channel 2
0	hc1_en_r	0	Enable Health Channel 1

Table 23. SET1 PM_SEL (ADDR 28h)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	pm_sel_r<2>	0	Select active LRHB channels:	000 --> LRHB1 data from CH1; LRHB2 OFF
5	pm_sel_r<1>	0		001 --> LRHB1 data from CH2; LRHB2 OFF
4	pm_sel_r<0>	0		010 --> LRHB1 data from CH3; LRHB2 OFF
				011 --> LRHB1 data from CH1; LRHB2 data from CH2
				100 --> LRHB1 data from CH1; LRHB2 data from CH3
				101 --> LRHB1 data from CH2; LRHB2 data from CH3
				110 --> LRHB1 OFF; LRHB2 OFF
				111 --> LRHB1 OFF; LRHB2 OFF
3	hc3_curinj_en_r	0	Enable health channel 3 current injection	
2	hc2_curinj_en_r	0	Enable health channel 2 current injection	
1	hc1_curinj_en_r	0	Enable health channel 1 current injection	
0	rld_en_r	0	Enable RLD driver	

Table 24. SET 2 AVG_CTRL (ADDR 29h)

BIT	Name	Default	Description	Configurations
7	avg_numb_buf_r<3>	0	Number of AVG buffers used in the system, this determines the compensation capacitance	0000 --> 0
6	avg_numb_buf_r<2>	0		0001 --> 1
5	avg_numb_buf_r<1>	0		0010 --> 2
4	avg_numb_buf_r<0>	0		0011 --> 3
			 1111 --> 15
3	avg_en_buf4_r	0	Enable AVG buffer 4	
2	avg_en_buf3_r	0	Enable AVG buffer 3	
1	avg_en_buf2_r	0	Enable AVG buffer 2	
0	avg_en_buf1_r	0	Enable AVG buffer 1	

Table 25. SET3 INCON_HCSEL_1 (2Ah)

BIT	Name	Default	Description	Configurations
7	ndev_bit1	0	Number of devices in application:	00 --> 1 device
6	ndev_bit0	0		01 --> 2 devices
				10 --> 3 devices
				11 --> 4 devices
5	inputcon_in1n_hcsel_r<2>	1	Connect input pad IN1N to one of the 6 health channel inputs	000 --> CH1 positive
4	inputcon_in1n_hcsel_r<1>	1		001 --> CH1 negative
3	inputcon_in1n_hcsel_r<0>	1		010 --> CH2 positive
				011 --> CH2 negative
				100 --> CH3 positive
				101 --> CH3 negative
				110 --> unconnected
				111 --> unconnected
2	inputcon_in1p_hcsel_r<2>	1	Connect input pad IN1P to one of the 6 channel inputs	Same setting of inputcon_in1n_hcsel_r
1	inputcon_in1p_hcsel_r<1>	1		
0	inputcon_in1p_hcsel_r<0>	1		

Table 26. SET4 INCON_HCSEL_2 (2Bh)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	DUMMY	0		
5	inputcon_in2n_hcsel_r<2>	1	Connect input pad IN2N to one of the 6 health channel inputs	Same setting of inputcon_in1n_hcsel_r
4	inputcon_in2n_hcsel_r<1>	1		
3	inputcon_in2n_hcsel_r<0>	1		
2	inputcon_in2p_hcsel_r<2>	1	Connect input pad IN2P to one of the 6 health channel inputs	Same setting of inputcon_in1n_hcsel_r
1	inputcon_in2p_hcsel_r<1>	1		
0	inputcon_in2p_hcsel_r<0>	1		

Table 27. SET5 INCON_HCSEL_3 (2Ch)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	DUMMY	0		
5	inputcon_in3n_hcsel_r<2>	1	Connect input pad IN3N to one of the 6 health channel inputs	Same setting of inputcon_in1n_hcsel_r
4	inputcon_in3n_hcsel_r<1>	1		
3	inputcon_in3n_hcsel_r<0>	1		
2	inputcon_in3p_hcsel_r<2>	1	Connect input pad IN3P to one of the 6 health channel inputs	Same setting of inputcon_in1n_hcsel_r
1	inputcon_in3p_hcsel_r<1>	1		
0	inputcon_in3p_hcsel_r<0>	1		

Table 28. SET6 INCON_AVG_1 (2Dh)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	DUMMY	0		
5	inputcon_avg2_r<2>	1	Connect input AVG buffer2 to any of the 6 input pads INxy (x=1,2,3 y=P/N)	000 --> IN1P
4	inputcon_avg2_r<1>	1		001 --> IN1N
3	inputcon_avg2_r<0>	1		010 --> IN2P
				011 --> IN2N
				100 --> IN3P
				101 --> IN3N
				110 --> unconnected
				111 --> unconnected
2	inputcon_avg1_r<2>	1	Connect input AVG buffer1 to any of the 6 input pads INxy (x=1,2,3 y=P/N)	Same setting of inputcon_avg2_r
1	inputcon_avg1_r<1>	1		
0	inputcon_avg1_r<0>	1		

Table 29. SET7 INCON_AVG_2 (2Eh)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	DUMMY	0		
5	inputcon_avg4_r<2>	1	Connect input AVG buffer4 to any of the 6 input pads INxy (x=1,2,3 y=P/N)	Same setting of inputcon_avg2_r
4	inputcon_avg4_r<1>	1		
3	inputcon_avg4_r<0>	1		
2	inputcon_avg3_r<2>	1	Connect input AVG buffer3 to any of the 6 input pads INxy (x=1,2,3 y=P/N)	Same setting of inputcon_avg2_r
1	inputcon_avg3_r<1>	1		
0	inputcon_avg3_r<0>	1		

Table 30. SET8 INCON_RLD (2Fh)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	ckext_en	0	Enable clock output	0: no clock out on ckext pin 1: clock out on ckext pin
5	clk_sel_r<1>	0	Select the internal, external or XTAL oscillator	00 --> Ring Oscillator
4	clk_sel_r<0>	0		01 --> Xtal Oscillator
				10 --> External clock
3	psmon_sel_r	1	Change the Common mode voltage of INA.	0-> VREF=0.7V To use when supply voltage is lower than 2V, typical 1.8V
				1-> VREF=1,0V To use when supply voltage is higher than 2V, typical 3.3V.
2	inputcon_rld_sel_r<2>	1	Connect the RLD output to any of the inputs pads INxN/P, for x=1,2,3	000 --> IN1P
1	inputcon_rld_sel_r<1>	1		001 --> IN1N
0	inputcon_rld_sel_r<0>	1		010 --> IN2P
				011 --> IN2N
				100 --> IN3P
			101 --> IN3N	
			110 --> unconnected	
			111 --> unconnected	

Table 31. SET9 CCK_EN_1 (30h)

BIT	Name	Default	Description	Configurations
7	In2n_contact_pdn_r	0	Contact check enable signal for N-side of DC contact check connected to in IN2N	0: current off 1: current on
6	In2n_contact_pdp_r	0	Contact check enable signal for P-side of DC contact check connected to IN2N	Same as IN2N_contact_en_r
5	In2p_contact_pdn_r	0	Contact check enable signal for N-side of DC contact check connected to IN2P	
4	In2p_contact_pdp_r	0	Contact check enable signal for P-side of DC contact check connected to IN2P	
3	In1n_contact_pdn_r	0	Contact check enable signal for N-side of DC contact check connected to IN1N	
2	In1n_contact_pdp_r	0	Contact check enable signal for P-side of DC contact check connected to IN1N	
1	in1p_contact_pdn_r	0	Contact check enable signal for N-side of DC contact check connected to IN1P	
0	in1p_contact_pdp_r	0	Contact check enable signal for P-side of DC contact check connected to IN1P	

Table 32. SET10 CCK_EN_2 (31h)

BIT	Name	Default	Description	Configurations
7	in1n_cont_cur_r<1>	0	Select the current (25/50/100/200nA) of the contact check connected to IN1N	00 --> 25 nA
6	in1n_cont_cur_r<0>	0		01 --> 50 nA
				10 --> 100 nA
				11 --> 200 nA
5	in1p_cont_cur_r<1>	0	Select the current (25/50/100/200nA) of the contact check connected to IN1P	Same setting of in1n_cont_cur_r
4	in1p_cont_cur_r<0>	0		
3	in3n_contact_pdn_r	0	Contact check enable signal for N-side of DC contact check connected to IN3N	
2	in3n_contact_pdp_r	0	Contact check enable signal for P-side of DC contact check connected to IN3N	
1	in3p_contact_pdn_r	0	Contact check enable signal for N-side of DC contact check connected to IN3P	
0	in3p_contact_pdp_r	0	Contact check enable signal for P-side of DC contact check connected to IN3P	

Table 33. SET11 CCK_CUR (32h)

BIT	Name	Default	Description	Configurations
7	in3n_cont_cur_r<1>	0	Select the current (25/50/100/200nA) of the contact check connected to IN3N	Same setting of in1n_cont_cur_r
6	in3n_cont_cur_r<0>	0		
5	in3p_cont_cur_r<1>	0	Select the current (25/50/100/200nA) of the contact check connected to IN3P	Same setting of in1n_cont_cur_r
4	in3p_cont_cur_r<0>	0		
3	in2n_cont_cur_r<1>	0	Select the current (25/50/100/200nA) of the contact check connected to IN2N	Same setting of in1n_cont_cur_r
2	in2n_cont_cur_r<0>	0		
1	in2p_cont_cur_r<1>	0	Select the current (25/50/100/200nA) of the contact check connected to IN2P	Same setting of in1n_cont_cur_r
0	in2p_cont_cur_r<0>	0		

Table 34. SET12 CCK_TRSH (33h)

BIT	Name	Default	Description	Configurations
7	cck_threshp_sel_r<3>	0	Select threshold at the Vdd side for the DC contact at ALL inputs (typical values)	0000 --> VDD-60uV
6	cck_threshp_sel_r<2>	0		0001 --> VDD-102mV
5	cck_threshp_sel_r<1>	0		0010 --> VDD-204 mV
4	cck_threshp_sel_r<0>	0		0011 --> VDD-306mV
				0100 --> VDD-408 mV
				0101 --> VDD-510mV
				0110 --> VDD-612mV
				0111 --> VDD-714mV
				1000 --> VDD-816mV
				1001 --> VDD-918mV
				1010 --> VDD-1.020 V
				1011 --> VDD- 1.122 V
				1100 --> VDD-1.224 V
				1101 --> VDD-1.326 V
				1110 --> VDD-1.427 V
				1111 --> VDD-1.529 V
3	cck_threshn_sel_r<3>	0	Select threshold at the V _{SS} side for the DC contact at ALL inputs (typical values)	0000 --> 60uV
2	cck_threshn_sel_r<2>	0		0001 --> 102mV
1	cck_threshn_sel_r<1>	0		0010 --> 204 mV
0	cck_threshn_sel_r<0>	0		0011 --> 306mV
				0100 --> 408 mV
				0101 --> 510mV
				0110 --> 612mV
				0111 --> 714mV
				1000 --> 816mV
				1001 --> 918mV
				1010 --> 1.020 V
				1011 --> 1.122 V
			1100 --> 1.224 V	
			1101 --> 1.326 V	
			1110 --> 1. 427 V	

Table 35. SET13 HC_ANA_CTRL (34h)

BIT	Name	Default	Description	Configurations
7	dataout_prefilter_en	0	Enable for data out pre-filter	
6	hc_pga_gain_r<1>	1	Select the gain of the PGA (1, 2, 4) for ALL health channels	00 --> 4
5	hc_pga_gain_r<0>	1		01 --> 2
				10 --> 4/3
				11 --> 1
4	hc_ina_gain_r<1>	0	Select the gain of the INA (8 or 16) for ALL health channels	00 --> 8
3	hc_ina_gain_r<0>	0		01 --> 8
				10 --> 16
				11 --> 16
2	hc_curinj_freq_r	0	Select the current injection frequency (2,5kHz or 5kHz) for ALL health channels	0 --> 2.5 kHz
				1 --> 5 kHz
1	hc_curinj_cur_r<1>	0	Select the current injection (5uA, 10uA or 20uA) ALL health channels	00 --> 5 μ A
0	hc_curinj_cur_r<0>	0		01 --> 10 μ A
				10 --> 20 μ A

Table 36. SET14 IMP_ANA_CTRL (35h)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	imp_ina_gain_r<1>	0	Select the gain of the INA (8 or 16) for the impedance channel	00 --> 8
5	imp_ina_gain_r<0>	0		01 --> 8
				10 --> 16
				11 --> 16
4	imp_curinj_cur_r<1>	0	Select the current injection (5 μ A, 10 μ A or 20 μ A) impedance channel	00 --> 5 μ A
3	imp_curinj_cur_r<0>	0		01 --> 10 μ A
				10 --> 20 μ A
2	imp_curinj_freq_r<2>	0	Select the current injection frequency. This is equal to the chopping frequency	000 --> fchop = 20 kHz
1	imp_curinj_freq_r<1>	0		001 --> fchop = 25 kHz
0	imp_curinj_freq_r<0>	0		010 --> fchop = 31.25 kHz
				011 --> fchop = 35.714 kHz
				100 --> fchop = 41.667 kHz
				101 --> fchop = 45.455 kHz
				110 --> fchop = 50 kHz

Table 37. SET15 ECG_DIGFILT_CTRL (36h)

BIT	Name	Default	Description	Configurations
7	hc_dig_ecghpf_sel_r<2>	1	Digital HPF cut-off frequency selection for the HRLB signal of ALL health channels. These settings are active when the <i>Recovery</i> mode is ON.	000 --> 5 Hz
6	hc_dig_ecghpf_sel_r<1>	1		001 --> 2 Hz
5	hc_dig_ecghpf_sel_r<0>	0		010 --> 1 Hz
				011 --> 0.7 Hz
				100 --> 0.5 Hz
				101 --> 0.1 Hz
				110--> 0.05 Hz
4	hc_dig_ecglpf_sel_r<3>	0	Digital LPF cut-off frequency selection for the HRLB signal of ALL health channels.	1000 --> 600 Hz
3	hc_dig_ecglpf_sel_r<2>	0		0000 --> 300 Hz
2	hc_dig_ecglpf_sel_r<1>	0		0001 --> 200 Hz
1	hc_dig_ecglpf_sel_r<0>	0		0010 --> 150 Hz
				0011 --> 100 Hz
				0100 --> 75 Hz
				0101 --> 50 Hz
			0110 --> 37.5 Hz	
			0111 --> 25 Hz	
0	DUMMY	0		

Table 38. SET16 PM_DIGFILT_CTRL (37h)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	imp_pga_gain_r<1>	0	Select the gain of the PGA (1, 2, 4) for the impedance channel	00 --> 4
5	imp_pga_gain_r<0>	0		01 --> 2
				10 --> 4/3
4	DUMMY	0		11 --> 1
3	hc_dig_pmhpf_sel_r<2>	0	Digital HPF cut-off frequency selection for the LRHB signal of ALL health channels. These settings are active when the <i>Recovery</i> mode is ON.	000 --> 5 Hz
2	hc_dig_pmhpf_sel_r<1>	1		001 --> 1 Hz
1	hc_dig_pmhpf_sel_r<0>	1		010 --> 0.7 Hz
				011 --> 0.05 Hz
				100 --> 1 kHz
0	hc_dig_pmlpf_sel_r	0	Digital LPF cut-off frequency selection for the LRHB signal of ALL health channels.	0 --> 10 kHz
				1 --> 5 kHz

Table 39. SET17 HC_DIGFILT_CTRL (38h)

BIT	Name	Default	Description	Configurations
7	hc3_dig_hpf_sel_r<2>	0	Digital HP cut off frequency for health channel 3. These settings are active when the <i>Recovery</i> mode is OFF	000 --> HRLB = 5Hz; LRHB = 5Hz
6	hc3_dig_hpf_sel_r<1>	0		001 --> HRLB = 2Hz; LRHB = 1Hz
5	hc3_dig_hpf_sel_r<0>	0		010 --> HRLB = 1Hz; LRHB = 1Hz
				011 --> HRLB = 0.7Hz; LRHB = 0.7Hz
				100 --> HRLB = 0.5Hz; LRHB = 0.7Hz
				101 --> HRLB = 0.1Hz; LRHB = 0.05Hz
				110 --> HRLB = 0.05Hz; LRHB = 0.05Hz
4	hc2_dig_hpf_sel_r<2>	0	Digital HP cut off frequency for health channel 2.	Same setting of hc3_dig_hpf_sel_r
3	hc2_dig_hpf_sel_r<1>	0	These settings are active when the <i>Recovery</i> mode is OFF	
2	hc2_dig_hpf_sel_r<0>	0		
1	hc1_dig_hpf_sel_r<2>	0	Digital HP cut off frequency for health channel 1.	Same setting of hc3_dig_hpf_sel_r
0	hc1_dig_hpf_sel_r<1>	0	These settings are active when the <i>Recovery</i> mode is OFF	

Table 40. SET18 HC_HPFAANA_CTRL (39h)

BIT	Name	Default	Description	Configurations
7	hc1_dig_hpf_sel_r<0>	0		
6	DUMMY	0		
5	hc3_rhpf_sel_r<1>	0	Select cut-off frequency of analog filter connected to HC3.	00 --> 5Hz
4	hc3_rhpf_sel_r<0>	0	These settings are active when the <i>Recovery</i> mode is OFF. When <i>Recovery</i> mode is ON they are set at 0.05Hz.	01 --> 0.7Hz
				10 --> 0.05Hz
				11 --> 0.05Hz
3	hc2_rhpf_sel_r<1>	0	Select cut-off frequency of analog filter connected to HC2.	Same setting of hc3_rhpf_sel_r
2	hc2_rhpf_sel_r<0>	0	These settings are active when the <i>Recovery</i> mode is OFF. When <i>Recovery</i> mode is ON they are set at 0.05Hz.	
1	hc1_rhpf_sel_r<1>	0	Select cut-off frequency of analog filter connected to HC1.	Same setting of hc3_rhpf_sel_r
0	hc1_rhpf_sel_r<0>	0	These settings are active when the <i>Recovery</i> mode is OFF. When <i>Recovery</i> mode is ON they are set at 0.05Hz.	

Table 41. SET19 RLD_CTRL (3Ah)

BIT	Name	Default	Description	Configurations
7	hc3_phaserev_r	0	Reverse the phase of the injection frequency of health channel 3. Used in unipolar measurements.	
6	hc2_phaserev_r	0	Reverse the phase of the injection frequency of health channel 2. Used in unipolar measurements.	
5	hc1_phaserev_r	0	Reverse the phase of the injection frequency of health channel 1. Used in unipolar measurements.	
4	rld_ref_sel_r<1>	0	Select reference for RLD	00 --> 0.7 V
3	rld_ref_sel_r<0>	0		01 --> 1 V
				10 --> 1.49 V
2	vref_sel_r	0	Register to select internal or external reference. 0->external reference; 1-> internal reference	
1	rld_cut_r	0	Register to cut or close RLD loop	0 --> Closed
				1 --> Open
0	imp_dig_lpf_sel_r	0	Digital LPF cut-off frequency selection for impedance channel	0 --> 20 Hz
				1 --> 1 Hz

Table 42. SET20 RECOVERY_TIME (3Bh)

BIT	Name	Default	Description	Configurations
7	DUMMY	0		
6	DUMMY	0		
5	DUMMY	0		
4	recovery_time_r<3>	0	Select the blanking time for overflow detection in steps of 2,5 ms. From 2,5 till 37,5ms. Can be put OFF as well.	0000 --> 2.5 ms
3	recovery_time_r<2>	0		0001 --> 5 ms
2	recovery_time_r<1>	0		0010 --> 7.5 ms
1	recovery_time_r<0>	0		0011 --> 10 ms
				0100 --> 12.5 ms
				0101 --> 15 ms
				0110 --> 17.5 ms
				0111 --> 20 ms
				1000 --> 22.5 ms
				1001 --> 25 ms
				1010 --> 27.5 ms
				1011 --> 30 ms
				1100 --> 32.5 ms
				1101 --> 35 ms
			1110 --> 37.5 ms	
			1111 --> Recovery Mode OFF	
0	hc_pmd_thres_r<8>	0	Pacemaker detection threshold	

Table 43. SET21 PMD_TRSH (3Ch)

BIT	Name	Default	Description	Configurations
7	hc_pmd_thres_r<7>	0	Pacemaker detection threshold	
6	hc_pmd_thres_r<6>	0		
5	hc_pmd_thres_r<5>	0		
4	hc_pmd_thres_r<4>	0		
3	hc_pmd_thres_r<3>	0		
2	hc_pmd_thres_r<2>	0		
1	hc_pmd_thres_r<1>	0		
0	hc_pmd_thres_r<0>	0		

Table 44. SET22 FILTER_SWTIME (3Dh)

BIT	Name	Default	Description	Configurations
7	Meas_mode	0	Measurement mode selection	0-> packets_streaming 1-> read data command
6	settings_ok_r	0	Starts measurement mode	
5	filter_swchtime2_r<2>	0	Select the switching time for the 2nd cut-off frequency step 0,7Hz-0,05Hz	000 --> 200 ms
4	filter_swchtime2_r<1>	0		001 --> 400 ms
3	filter_swchtime2_r<0>	0		010 --> 600 ms
				011 --> 800 ms
				100 to 111 --> 1 s
2	filter_swchtime1_r<2>	0	Select the switching time for the first cut-off frequency step 5Hz-0,7Hz	Same setting of filter_swchtime2_r
1	filter_swchtime1_r<1>	0		
0	filter_swchtime1_r<0>	0		

Table 45. SET23 DIGIO_IO (40h)

BIT	Name	Default	Description
7	DUMMY	0	
6	DUMMY	0	
5	DUMMY	0	
4	DUMMY	0	
3	DUMMY	0	
2	digio2_config_r	1	To configure DIGIOx in input or output mode 0: input; 1: output
1	digio1_config_r	1	
0	digio0_config_r	1	

Table 46. SET24 IMP_CUR_EN (44h)

BIT	Name	Default	Description
7	DUMMY	0	
6	imp_curinj_en_r	1	Enable impedance current injection (CIP, CIN current generators)
5	Reserved	0	
4	Reserved	0	
3	Reserved	0	
2	Reserved	0	
1	Reserved	0	
0	Reserved	0	

Table 47. SET25 DIGIO12_SEL (45h)

BIT	Name	Default	Description
7	Digio2_muxsel_r<3>	0	Select input signal for DIGIO2
6	Digio2_muxsel_r<2>	0	
5	Digio2_muxsel_r<1>	0	
4	Digio2_muxsel_r<0>	0	
3	Digio1_muxsel_r<3>	0	Select input signal for DIGIO1
2	Digio1_muxsel_r<2>	0	
1	Digio1_muxsel_r<1>	0	
0	Digio1_muxsel_r<0>	0	

Table 48. SET26 DIGIO0_SEL (46h)

BIT	Name	Default	Description
7	Digio0_muxsel_r<3>	0	Select input signal for DIGIO0
6	Digio0_muxsel_r<2>	0	
5	Digio0_muxsel_r<1>	0	
4	Digio0_muxsel_r<0>	0	
3	DUMMY	0	
2	DUMMY	0	
1	DUMMY	0	
0	DUMMY	0	

6.12.2 Output flags (read only)

Table 49. OUT_FLAG0 (47h)

BIT	Name	Def.	Description
7	DUMMY		
6	imp_overflow_r	0	Impedance Channel is in overflow mode
5	hc3_overflow_r	0	Channel 3 is in overflow mode
4	hc2_overflow_r	0	Channel 2 is in overflow mode
3	hc1_overflow_r	0	Channel 1 is in overflow mode
2	DUMMY	0	
1	DUMMY	0	
0	DUMMY	0	

Table 50. OUT_FLAG1 (48h)

BIT	Name	Def.	Description
7	psmon_out_r<1>	0	
6	psmon_out_r<0>	0	
5	ln3n_contact_out_r	0	IN3N has bad contact. This is an OR of in3n_contact_outp_i & in3n_contact_outn_i
4	ln3p_contact_out_r	0	IN3P has bad contact. This is an OR of in3p_contact_outp_i & in3p_contact_outn_i
3	ln2n_contact_out_r	0	IN2N has bad contact. This is an OR of in2n_contact_outp_i & in2n_contact_outn_i
2	ln2p_contact_out_r	0	IN2P has bad contact. This is an OR of in2p_contact_outp_i & in2p_contact_outn_i
1	in1n_contact_out_r	0	IN1N has bad contact. This is an OR of in1n_contact_outp_i & in1n_contact_outn_i
0	in1p_contact_out_r	0	IN1P has bad contact. This is an OR of in1p_contact_outp_i & in1p_contact_outn_i

6.12.3 Data registers (readable only if MEAS_MODE = 1)

Table 51. ECG1_DATAOUT_1 (49h)

BIT	Name	Def.	Description
7	ecg1_dataout_r<15>	0	MSB of HRLB channel 1. This register contains the Most Significant Byte of the output data from the HRLB1 channel and it is readable when Meas_Mode=1
6	ecg1_dataout_r<14>	0	
5	ecg1_dataout_r<13>	0	
4	ecg1_dataout_r<12>	0	
3	ecg1_dataout_r<11>	0	
2	ecg1_dataout_r<10>	0	
1	ecg1_dataout_r<9>	0	
0	ecg1_dataout_r<8>	0	

Table 52. CG1_DATAOUT_0 (4Ah)

BIT	Name	Def.	Description
7	ecg1_dataout_r<7>	0	LSB of HRLB channel 1. This register contains the Least Significant Byte of the output data from the HRLB1 channel and it is readable when Meas_Mode=1
6	ecg1_dataout_r<6>	0	
5	ecg1_dataout_r<5>	0	
4	ecg1_dataout_r<4>	0	
3	ecg1_dataout_r<3>	0	
2	ecg1_dataout_r<2>	0	
1	ecg1_dataout_r<1>	0	
0	ecg1_dataout_r<0>	0	

Table 53. ECG2_DATAOUT_1 (4Bh)

BIT	Name	Def.	Description
7	ecg2_dataout_r<15>	0	MSB of HRLB channel 2. This register contains the Most Significant Byte of the output data from the HRLB2 channel and it is readable when Meas_Mode=1
6	ecg2_dataout_r<14>	0	
5	ecg2_dataout_r<13>	0	
4	ecg2_dataout_r<12>	0	
3	ecg2_dataout_r<11>	0	
2	ecg2_dataout_r<10>	0	
1	ecg2_dataout_r<9>	0	
0	ecg2_dataout_r<8>	0	

Table 54. ECG2_DATAOUT_0 (4Ch)

BIT	Name	Def.	Description
7	ecg2_dataout_r<7>	0	LSB of HRLB channel 2. This register contains the Least Significant Byte of the output data from the HRLB2 channel and it is readable when Meas_Mode=1
6	ecg2_dataout_r<6>	0	
5	ecg2_dataout_r<5>	0	
4	ecg2_dataout_r<4>	0	
3	ecg2_dataout_r<3>	0	
2	ecg2_dataout_r<2>	0	
1	ecg2_dataout_r<1>	0	
0	ecg2_dataout_r<0>	0	

Table 55. ECG3_DATAOUT_1 (4Dh)

BIT	Name	Def.	Description
7	ecg3_dataout_r<15>	0	MSB of HRLB channel 3. This register contains the Most Significant Byte of the output data from the HRLB3 channel and it is readable when Meas_Mode=1
6	ecg3_dataout_r<14>	0	
5	ecg3_dataout_r<13>	0	
4	ecg3_dataout_r<12>	0	
3	ecg3_dataout_r<11>	0	
2	ecg3_dataout_r<10>	0	
1	ecg3_dataout_r<9>	0	
0	ecg3_dataout_r<8>	0	

Table 56. ECG3_DATAOUT_0 (4Eh)

BIT	Name	Def.	Description
7	ecg3_dataout_r<7>	0	LSB of HRLB channel 3. This register contains the Least Significant Byte of the output data from the HRLB3 channel and it is readable when Meas_Mode=1
6	ecg3_dataout_r<6>	0	
5	ecg3_dataout_r<5>	0	
4	ecg3_dataout_r<4>	0	
3	ecg3_dataout_r<3>	0	
2	ecg3_dataout_r<2>	0	
1	ecg3_dataout_r<1>	0	
0	ecg3_dataout_r<0>	0	

Table 57. ECG12_DATAOUT_1 (4Fh)

BIT	Name	Def.	Description
7	ecg12_dataout_r<15>	0	MSB of ECG12_dataout. This register contains the Most Significant Byte of the half sum between the output data from the ECG1 Chain and the output data from the ECG2 Chain and it is readable when Meas_Mode=1
6	ecg12_dataout_r<14>	0	
5	ecg12_dataout_r<13>	0	
4	ecg12_dataout_r<12>	0	
3	ecg12_dataout_r<11>	0	
2	ecg12_dataout_r<10>	0	
1	ecg12_dataout_r<9>	0	
0	ecg12_dataout_r<8>	0	

Table 58. ECG12_DATAOUT_0 (50h)

BIT	Name	Def.	Description
7	ecg12_dataout_r<7>	0	LSB of ECG12_dataout. This register contains the Least Significant Byte of the half sum between the output data from the ECG1 Chain and the output data from the ECG2 Chain and it is readable when Meas_Mode=1
6	ecg12_dataout_r<6>	0	
5	ecg12_dataout_r<5>	0	
4	ecg12_dataout_r<4>	0	
3	ecg12_dataout_r<3>	0	
2	ecg12_dataout_r<2>	0	
1	ecg12_dataout_r<1>	0	
0	ecg12_dataout_r<0>	0	

Table 59. ECG23_DATAOUT_1 (51h)

BIT	Name	Def.	Description
7	ecg23_dataout_r<15>	0	MSB of ECG23_dataout. This register contains the Most Significant Byte of the half sum between the output data from the ECG2 Chain and the output data from the ECG3 Chain and it is readable when Meas_Mode=1
6	ecg23_dataout_r<14>	0	
5	ecg23_dataout_r<13>	0	
4	ecg23_dataout_r<12>	0	
3	ecg23_dataout_r<11>	0	
2	ecg23_dataout_r<10>	0	
1	ecg23_dataout_r<9>	0	
0	ecg23_dataout_r<8>	0	

Table 60. ECG23_DATAOUT_0 (52h)

BIT	Name	Def.	Description
7	ecg23_dataout_r<7>	0	LSB of ECG23_dataout. This register contains the Least Significant Byte of the half sum between the output data from the ECG2 Chain and the output data from the ECG3 Chain and it is readable when Meas_Mode=1
6	ecg23_dataout_r<6>	0	
5	ecg23_dataout_r<5>	0	
4	ecg23_dataout_r<4>	0	
3	ecg23_dataout_r<3>	0	
2	ecg23_dataout_r<2>	0	
1	ecg23_dataout_r<1>	0	
0	ecg23_dataout_r<0>	0	

Table 61. ECG31_DATAOUT_1 (53h)

BIT	Name	Def.	Description
7	ecg31_dataout_r<15>	0	MSB of ECG31_dataout. This register contains the Most Significant Byte of the half sum between the output data from the ECG3 Chain and the output data from the ECG1 Chain and it is readable when Meas_Mode=1
6	ecg31_dataout_r<14>	0	
5	ecg31_dataout_r<13>	0	
4	ecg31_dataout_r<12>	0	
3	ecg31_dataout_r<11>	0	
2	ecg31_dataout_r<10>	0	
1	ecg31_dataout_r<9>	0	
0	ecg31_dataout_r<8>	0	

Table 62. ECG31_DATAOUT_0 (54h)

BIT	Name	Def.	Description
7	ecg31_dataout_r<7>	0	LSB of ECG31_dataout. This register contains the Least Significant Byte of the half sum between the output data from the ECG3 Chain and the output data from the ECG1 Chain and it is readable when Meas_Mode=1
6	ecg31_dataout_r<6>	0	
5	ecg31_dataout_r<5>	0	
4	ecg31_dataout_r<4>	0	
3	ecg31_dataout_r<3>	0	
2	ecg31_dataout_r<2>	0	
1	ecg31_dataout_r<1>	0	
0	ecg31_dataout_r<0>	0	

Table 63. PM1_DATAOUT_1 (55h)

BIT	Name	Def.	Description
7	pm1_dataout_r<15>	0	MSB of LRHB channel 1. This register contains the Most Significant Byte of the output data from the LRHB 1 channel and it is readable when Meas_Mode=1
6	pm1_dataout_r<14>	0	
5	pm1_dataout_r<13>	0	
4	pm1_dataout_r<12>	0	
3	pm1_dataout_r<11>	0	
2	pm1_dataout_r<10>	0	
1	pm1_dataout_r<9>	0	
0	pm1_dataout_r<8>	0	

Table 64. PM1_DATAOUT_0 (56h)

BIT	Name	Def.	Description
7	pm1_dataout_r<7>	0	LSB of LRHB channel 1. This register contains the Least Significant Byte of the output data from the LRHB1 channel and it is readable when Meas_Mode=1
6	pm1_dataout_r<6>	0	
5	pm1_dataout_r<5>	0	
4	pm1_dataout_r<4>	0	
3	pm1_dataout_r<3>	0	
2	pm1_dataout_r<2>	0	
1	pm1_dataout_r<1>	0	
0	pm1_dataout_r<0>	0	

Table 65. PM2_DATAOUT_1 (57h)

BIT	Name	Def.	Description
7	pm2_dataout_r<15>	0	MSB of LRHB channel 2. This register contains the Most Significant Byte of the output data from the LRHB2 channel and it is readable when Meas_Mode=1
6	pm2_dataout_r<14>	0	
5	pm2_dataout_r<13>	0	
4	pm2_dataout_r<12>	0	
3	pm2_dataout_r<11>	0	
2	pm2_dataout_r<10>	0	
1	pm2_dataout_r<9>	0	
0	pm2_dataout_r<8>	0	

Table 66. PM2_DATAOUT_0 (58h)

BIT	Name	Def.	Description
7	pm2_dataout_r<7>	0	LSB of LRHB channel 2. This register contains the Least Significant Byte of the output data from the LRHB2 channel and it is readable when Meas_Mode=1
6	pm2_dataout_r<6>	0	
5	pm2_dataout_r<5>	0	
4	pm2_dataout_r<4>	0	
3	pm2_dataout_r<3>	0	
2	pm2_dataout_r<2>	0	
1	pm2_dataout_r<1>	0	
0	pm2_dataout_r<0>	0	

Table 67. IMPEDANCE_PHASE_AC_DATAOUT_1 (59h)

BIT	Name	Def.	Description
7	impp_ac_dataout_r<15>	0	MSB of IMPP_AC_dataout. This register contains the Most Significant Byte of the output data from the IMPEDANCE PHASE AC and it is readable when Meas_Mode=1
6	impp_ac_dataout_r<14>	0	
5	impp_ac_dataout_r<13>	0	
4	impp_ac_dataout_r<12>	0	
3	impp_ac_dataout_r<11>	0	
2	impp_ac_dataout_r<10>	0	
1	impp_ac_dataout_r<9>	0	
0	impp_ac_dataout_r<8>	0	

Table 68. IMPEDANCE_PHASE_AC_DATAOUT_0 (5Ah)

BIT	Name	Def.	Description
7	impp_ac_dataout_r<7>	0	LSB of IMPP_AC_dataout. This register contains the Least Significant Byte of the output data from the IMPEDANCE PHASE AC and it is readable when Meas_Mode=1
6	impp_ac_dataout_r<6>	0	
5	impp_ac_dataout_r<5>	0	
4	impp_ac_dataout_r<4>	0	
3	impp_ac_dataout_r<3>	0	
2	impp_ac_dataout_r<2>	0	
1	impp_ac_dataout_r<1>	0	
0	impp_ac_dataout_r<0>	0	

Table 69. IMPEDANCE_SQUARING_AC_DATAOUT_1 (5Bh)

BIT	Name	Def.	Description
7	impq_ac_dataout_r<15>	0	MSB of IMPQ_AC_dataout. This register contains the Most Significant Byte of the output data from the IMPEDANCE SQUARING AC and it is readable when Meas_Mode=1
6	impq_ac_dataout_r<14>	0	
5	impq_ac_dataout_r<13>	0	
4	impq_ac_dataout_r<12>	0	
3	impq_ac_dataout_r<11>	0	
2	impq_ac_dataout_r<10>	0	
1	impq_ac_dataout_r<9>	0	
0	impq_ac_dataout_r<8>	0	

Table 70. IMPEDANCE_SQUARING_AC_DATAOUT_0 (5Ch)

BIT	Name	Def.	Description
7	impq_ac_dataout_r<7>	0	LSB of IMPP_AC_dataout. This register contains the Least Significant Byte of the output data from the IMPEDANCE SQUARING AC and it is readable when Meas_Mode=1
6	impq_ac_dataout_r<6>	0	
5	impq_ac_dataout_r<5>	0	
4	impq_ac_dataout_r<4>	0	
3	impq_ac_dataout_r<3>	0	
2	impq_ac_dataout_r<2>	0	
1	impq_ac_dataout_r<1>	0	
0	impq_ac_dataout_r<0>	0	

Table 71. IMPEDANCE_PHASE_DC_DATAOUT_1 (5Dh)

BIT	Name	Def.	Description
7	impp_dc_dataout_r<15>	0	MSB of IMPP_DC_dataout. This register contains the Most Significant Byte of the output data from the IMPEDANCE PHASE DC and it is readable when Meas_Mode=1
6	impp_dc_dataout_r<14>	0	
5	impp_dc_dataout_r<13>	0	
4	impp_dc_dataout_r<12>	0	
3	impp_dc_dataout_r<11>	0	
2	impp_dc_dataout_r<10>	0	
1	impp_dc_dataout_r<9>	0	
0	impp_dc_dataout_r<8>	0	

Table 72. IMPEDANCE_PHASE_DC_DATAOUT_0 (5Eh)

BIT	Name	Def.	Description
7	impp_dc_dataout_r<7>	0	LSB of IMPP_DC_dataout. This register contains the Least Significant Byte of the output data from the IMPEDANCE PHASE DC and it is readable when Meas_Mode=1
6	impp_dc_dataout_r<6>	0	
5	impp_dc_dataout_r<5>	0	
4	impp_dc_dataout_r<4>	0	
3	impp_dc_dataout_r<3>	0	
2	impp_dc_dataout_r<2>	0	
1	impp_dc_dataout_r<1>	0	
0	impp_dc_dataout_r<0>	0	

Table 73. IMPEDANCE_SQUARING_DC_DATAOUT_1 (5Fh)

BIT	Name	Def.	Description
7	impq_dc_dataout_r<15>	0	MSB of IMPQ_DC_dataout. This register contains the Most Significant Byte of the output data from the IMPEDANCE SQUARING DC and it is readable when Meas_Mode=1
6	impq_dc_dataout_r<14>	0	
5	impq_dc_dataout_r<13>	0	
4	impq_dc_dataout_r<12>	0	
3	impq_dc_dataout_r<11>	0	
2	impq_dc_dataout_r<10>	0	
1	impq_dc_dataout_r<9>	0	
0	impq_dc_dataout_r<8>	0	

Table 74. IMPEDANCE_SQUARING_DC_DATAOUT_0 (60h)

BIT	Name	Def.	Description
7	impq_dc_dataout_r<7>	0	LSB of IMPQ_DC_dataout. This register contains the Least Significant Byte of the output data from the IMPEDANCE SQUARING DC and it is readable when Meas_Mode=1
6	impq_dc_dataout_r<6>	0	
5	impq_dc_dataout_r<5>	0	
4	impq_dc_dataout_r<4>	0	
3	impq_dc_dataout_r<3>	0	
2	impq_dc_dataout_r<2>	0	
1	impq_dc_dataout_r<1>	0	
0	impq_dc_dataout_r<0>	0	

Table 75. CONTACT_CHECK_DATAOUT_1 (61h)

BIT	Name	Def.	Description
7	dummy	0	MSB of CC_dataout. This register contains the Most Significant Byte of the output data from the CONTACT CHECK and it is readable when Meas_Mode=1
6	dummy	0	
5	overcurr_p	0	
4	overcurr_n	0	
3	psmon1	0	
2	psmon0	0	
1	imp_overflow_flags	0	
0	hc_overflow_flag3	0	

Table 76. CONTACT_CHECK_DATAOUT_0 (62h)

BIT	Name	Def.	Description
7	hc_overflow_flag2	0	LSB of CC_dataout. This register contains the Least Significant Byte of the output data from the CONTACT CHECK and it is readable when Meas_Mode=1
6	hc_overflow_flag1	0	
5	in_contact_out_flag6	0	
4	in_contact_out_flag5	0	
3	in_contact_out_flag4	0	
2	in_contact_out_flag3	0	
1	in_contact_out_flag2	0	
0	in_contact_out_flag1	0	

6.13 Output data format

In order to optimize the communication between the HM301D and the microcontroller, the HM301D implements an automatic data transmission able to minimize the communication load. In order to read the device data, the MCU doesn't need to send the register addresses to the device but it is the HM301D which continuously sends the data to the MCU. These data are organized in a packet which presents an added header in order to describe the meaning of the data included inside the packet. Anyhow the MCU can stop the data flow by pulling up the CS pin anytime.

All the data values are in binary twos complement format. The table below shows the ideal codes:

Table 77. Data format

Input Signal	Ideal Output Code
$\geq V_{REF}/GAIN$	7FFFh
$+V_{REF}/GAIN/(2^{15}-1)$	0001h
0	0000h
$-V_{REF}/GAIN/(2^{15}-1)$	FFFFh
$\leq -V_{REF}/GAIN/(2^{15}-(2^{15}-1))$	8000h

The HM301D can send the processed data of biopotential channels and impedance channel or the raw data of the biopotential channels just after the first decimation filters (see Figure 4).

The data packet is different according to the type of data that is transmitted.

6.13.1 Case 1: complete processed data - 4x packet

In this case the packet will be formed by four words of 16 bits each (base packet). In case of multi-chip configuration each device provides its own base packet. Those base packets are organized in the following way.

Table 78. Base packet

16 bits	16 bits	16 bits	16 bits
HEADER	C_DATA	LRHB1_DATA	LRHB2_DATA

where the c_data can be a biopotential data vector or an impedance data vector or a miscellaneous data vector. In multi-chip configuration, the packet that the MCU receives contains first the header base packet for each device, then the c_data base packet for each device and so on. Of course the first packet the MCU receives is sent by the last device in the chain and so on. For instance, if there are three devices in chain the order of the base packets inside the complete packet is:

Table 79. Data packet out with 3 HM301D in chain

HEADE R S3	HEADE R S2	HEADE R S1	C_DAT A S3	C_DAT A S2	C_DAT A S1	LRHB1 S3	LRHB1 S2	LRHB1 S1	LRHB2 S3	LRHB S2	LRHB S1
---------------	---------------	---------------	---------------	---------------	---------------	-------------	-------------	-------------	-------------	------------	------------

For every kind of configuration, every complete packet is updated with the LRHB channel path frequency. This frequency is function of the filters setting and can be 31.25 kHz or 15.625 kHz.

In the following example we use the highest cut-off frequency ($f_c = 31.25$ kHz). Therefore, in the case of three devices in chain, to correctly transfer all the data from the devices to the MCU, a minimum serial clock frequency (fsck) is needed:

$$f_{sck} = N_{dev} * L_W * N_{pac} * f_{pm} = 3 * 16 * 4 * 31.25 \text{ kHz} = 6 \text{ MHz}$$

where:

N_{dev} : devices number in chain;

L_W : word length;

N_{pac} : number of words per device.

Since the LRHB channel paths are updated with much lower frequency than the HRLB ones, there are some null vectors. Another contribution to the null packets is given by if some channel is not used (e.g.: max number of pm signals per application).

In order to have a more clear idea of the maximum number of useful packets, we have to consider that the minimum ratio between the LRHB frequency and the HRLB frequency is 32 ($f_{pm} = 31.25 \text{ kHz}$) and the minimum ratio between the LRHB frequency and the impedance frequency is 200 (see par 0 for details). To get all the information about the biopotential channels we need to get 6 base packets (3 channels + 3 half-sums), therefore we obtain that 6 HRLB useful packets every 32 complete packets will be transferred.

For the impedance data, the device has to transfer 4 base_packets (IAC, QAC, IDC, QDC), therefore 4 useful packets every 200 complete packets will be transferred for the impedance channel.

6.13.2 Case 2: pre-filtered data out - 3x packet

In this case the complete packet will be composed by 3 base_packets for each device in chain. The above mentioned base_packets will be ordered in the following way:

Table 80. Pre-filtered data out

16 bits		16 bits		16 bits	
12 bits	4 bits	8 bits	8 bits	4 bits	12 bits
HEADER <11:0>	CH1 <11:8>	CH1 <7:0>	CH2 <11:4>	CH2 <3:0>	CH3 <11:0>

where: CH1, CH2 and CH3 are the 12 bits vectors at the first decimator output.

Of course if we have three devices in chain the packets will be ordered as the previous case. In this case, every device has to transfer three vectors of 12 bits.

Considering a configuration with 3 devices in chain the serial clock frequency (f_{sck}): needed to transfer all the data from the devices to the host is:

$$f_{sck} = N_{dev} * L_V * N_{pac} * f_{prefilt} = 3 * 16 * 3 * 125 \text{ kHz} = 18 \text{ MHz}$$

where:

N_{dev} : devices number in chain;

L_V : vectors length;

N_{pac} : packets number per device;

$f_{prefilt}$: pre-filtered data refresh frequency.

in the case of 1 device:

$$f_{sck} = N_{dev} * L_V * N_{pac} * f_{prefilt} = 1 * 16 * 3 * 125 \text{ kHz} = 6 \text{ MHz}$$

So, in the case of 1 device with just 1 enabled channel:

$$f_{sck} = N_{dev} * L_V * N_{pac} * f_{prefilt} = 1 * 16 * 2 * 125 \text{ kHz} = 4 \text{ MHz}$$

This is the minimum serial clock frequency (f_{sck}) needed to transfer a pre-filtered data vector for the minimum configuration (1 device with 1 enabled channel).

6.13.3 Header description

The header packet contains the useful info to correctly interpret the whole packet meaning. The header packet is composed by 16bits in case 1 and by 12 bits in case 2:

Table 81. Header packet bits description in 4x packet case

Header bits	Name	Description	Details
15:11		Not used	
10	LRHB2_EN	LRHB channel 2 data enable	
9	LRHB1_EN	LRHB channel 1 data enable	
8:7	NUM_DEV <2:0>	Number Devices in daisy chain configuration	00: 1 device
			01: 2 devices
			10: 3 devices
			11: 4 devices
6	PREFIL_EN	Pre-filtered data out enable	
5	PMD2	LRHB channel 2 data enable	
4	PMD1	LRHB channel 1 data enable	
3:0	C_DATA_DESC <3:0>	C_DATA description	See Table 82

Table 82. Header packet bits description in 3x packet case

Header bits	Name	Description	Details
11:9		Not used	
8:7	NUM_DEV <2:0>	Number Devices in daisy chain configuration	00: 1 device
			01: 2 devices
			10: 3 devices
			11: 4 devices
6	PREFIL_EN	Pre-filtered data out enable	
5	LRHB2_EN	LRHB channel 2 data enable	
4	LRHB1_EN	LRHB channel 1 data enable	
3:0	C_DATA_DESC <3:0>	C_DATA description	See Table 82

The C_DATA packet contains different data according to the C_DATA_DESC. This is valid only for 4x packet case because in 3x packet case just the channels data is provided and without any filtering.

Table 83. C_DATA packet description bits configurations

C_DATA_DESC	
[3:0]	C_DATA content
0000	No useful data in C_DATA vector
0001	CH1_HRLB data
0010	CH2_HRLB data
0011	CH3_HRLB data
0100	NOT USED
0101	(CH1_HRLB + CH2_HRLB)/2 data
0110	(CH2_HRLB + CH3_HRLB)/2 data
0111	(CH3_HRLB + CH1_HRLB)/2 data
1000	ZC DC_I data
1001	ZC DC_Q data
1010	ZC AC_I data
1011	ZC AC_Q data
1100	Contact Check and overflow data (See Table 82)
1101	NOT USED
1110	NOT USED
1111	NOT USED

When the C_DATA vector contains the contact check and overflow data, its 16 bits have the following meaning:

Table 84. Contact check and overflow C_DATA vector

Contact check and overflow C_DATA details [C_DATA_DESC=1100]	
<15:0>	Description
15:14	Not used
13	over_curr_p
12	over_curr_n
11:10	psmon
9	Impedance channel overflow
8	CH3 overflow
7	CH2 overflow

Table 84. Contact check and overflow C_DATA vector (continued)

Contact check and overflow C_DATA details [C_DATA_DESC=1100]	
<15:0>	Description
6	CH1 overflow
5	IN3N DC contact check
4	IN3P DC contact check
3	IN2N DC contact check
2	IN2P DC contact check
1	IN1N DC contact check
0	IN1P DC contact check

6.14 Data rate

The following two tables describe respectively the HRLB data-out sampling frequencies as function of the HRLB low pass filter cut-off frequency and the LRHB data-out sampling frequencies as function of the LRHB low pass filter cut-off frequency.

Also for the impedance channel the data rate is function of low pass filter cut-off frequency; [Table 87](#) provides the two sampling frequencies as function of low pass filter cut-off frequency.

Table 85. HRLB data-out sampling frequency vs low pass filter cut-off frequency

CiaHRLB low pass fcut selector [hc_dig_ecglpf_sel_r] in SET15 register	Low pass cut-off frequency (-3 dB)	Sampling frequency HRLB data out
1000	600 Hz	1.953 kHz
0000	300 Hz	0.976 kHz
0001	200 Hz	0.651 kHz
0010	150 Hz	0.488 kHz
0011	100 Hz	0.325 kHz
0100	75 Hz	0.244 kHz
0101	50 Hz	0.163 kHz
0110	37 Hz	0.122 kHz
0111	25 Hz	0.0815 kHz

Table 86. LRHB data-out sampling frequency vs low pass filter cut-off frequency

PM low pass f_{cut} selector [hc_dig_pmlpf_sel_r] in SET 16 register	Low pass cut-off frequency (-3 dB)	Sampling frequency PM data out
0	10 kHz	31.25 kHz
1	5 kHz	15.625 kHz

Table 87. Impedance data-out sampling frequency vs low pass filter cut-off frequency


Impedance low pass f_{cut} selector [imp_dig_lpf_sel_r] in SET19 register	Low pass cut-off frequency (-3 dB)	Sampling frequency Impedance data out
0	1 Hz	7.8 Hz
1	20 Hz	156 Hz

6.15 Data ready operation

The HM301D has two types of data ready and SPI clock operation: packets data streaming and direct read command mode. These two procedures can be selected by Meas_mode bit of SET22 register (SET22 <7>).

One of the two ways can be used by choosing the proper signal as data ready in one of the DGIOs (refer to [Table 11](#), [Table 12](#) and [Table 13](#)). The packets data streaming method must be used if we are interested to retrieve the LRHB data; in this case the data ready signal to monitor is the pm_rsh. If we are interested to read only the ECG data then the direct read command procedure must be selected and the data ready signal to monitor is the ecg_rsh.

Figure 21. SPI communication - packet data streaming

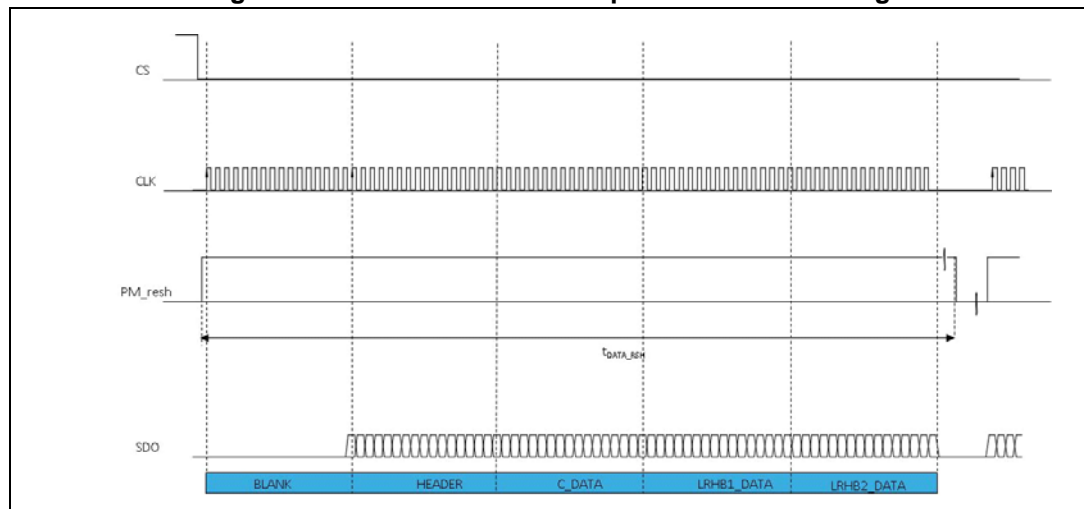

If Meas_mode bit is zero, the packets data streaming operation is selected. In case of complete processed data the packet is composed by 4 words of 16 bits and the SPI master must send at least 80 clock pulses only after the Pm_rsh signal goes high. The first 16 pulses are used by the HM301D to shift the data into the SPI registers so SDO stays low. While with the other 64 clock pulses the MCU can retrieve the 64bits packet data ([Figure 18](#)).


In case of pre-filtered data, the operation is exactly the same except for the fact that the packet is composed by 3 words bits so, just 64 and not 80 bits should be supplied by the MCU. In this case the right signal to be used as data ready is the prefilt_rsh which is output on DGIO0 with DGIO0_muxsel_r=1010 and on DGIO1 with DGIO1_muxsel_r=1001.

In both cases the tDATA_RSHB is set by the internal clock of the LRHB which can be 31.25 kHz or 15.625 kHz according to the low pass filter selection of the LRHB signal chain.

If just the HRLB signals are of interest, the data can be retrieved using the SPI data read command mode. To select this method the Meas_mode bit must be asserted. In this case

the ecg_rsh must be used as trigger signal, so when ecg_rsh goes high the microcontroller must directly read the ECG_OUT registers using the direct word reading procedure as described in [Figure 19](#). This ecg_rsh signal is available at DGIO2 with DGIO2_muxsel_r=1010.

Figure 22. ECG_OUT registers data reading

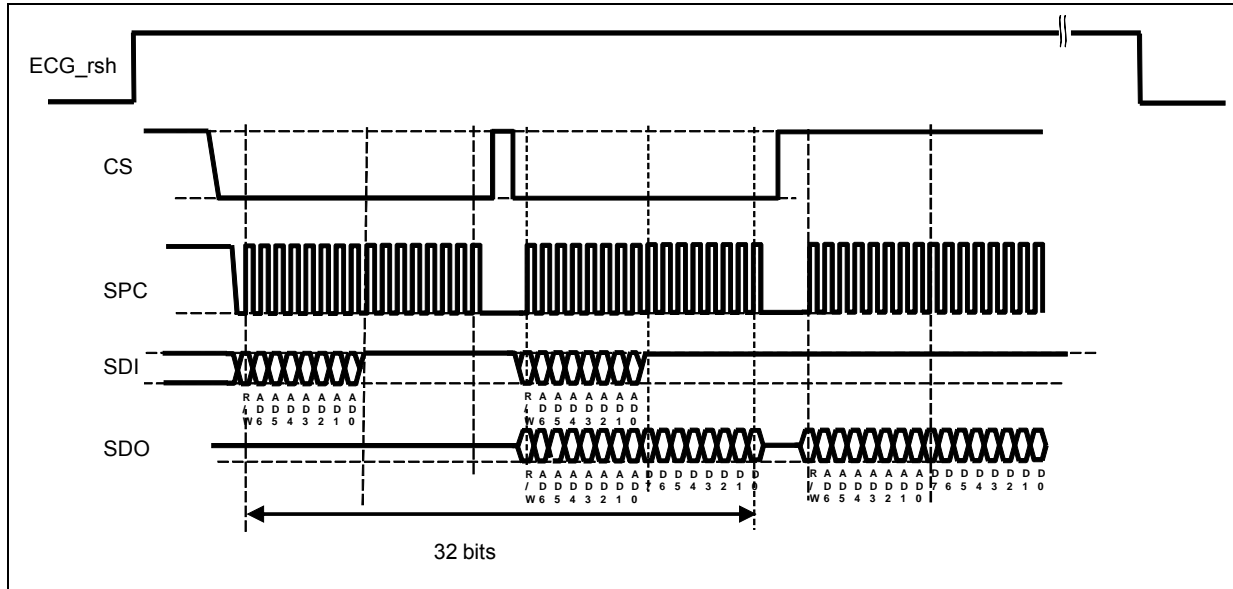

7 Application Information

7.1 DC offset removal

The electrode half-cell potential acts as a DC offset voltage on each of the incoming electrode signals and, depending on the application, also on the outgoing RLD electrode signal. In the biopotential channels and in the impedance channel the DC component is removed by the high pass filters.

The maximum half cell potential (DC_OS) the device can handle is defined by the supply voltage and by the RLD reference voltage RLF_VREF. Since the DC value is removed at the inputs of each acquisition channel, the limiting building block is the output swing of the RLD buffer which is limited by the supply voltage. The output swing towards VSS is limited by the difference between VREF and VSS. The output swing towards VDD is limited by the difference between VDD and RLF_VREF.

The worst case situation is when all half-cell potentials are in the same direction, i.e. positive or negative. In this case from the RLD output buffer towards the input of the health channel two half-cell potentials have to be subtracted. According to the medical standard, the RLD has to deliver 880 nA peak current. This gives an additional voltage drop of 264 mV over the DC current limiting resistor of the RLD. So the maximum output swing the RLD node (after the internal resistor) is VSS+325 mV and VDD-350 mV.

Taking all signals into account, the maximum DC offset can be calculated as the minimum of the following two equations:

Equation 3

$$DCOS_{VSS} = RLD_VREF - (VSS + 0.325)$$


Equation 4

$$DCOS_{VDD} = (VDD - 0.350) - RLD_VREF$$

For higher VDD, $DCOS_{VDD}$ increases while $DCOS_{VSS}$ stays the same. So, at high VDD, it is beneficial to increase the RLD reference voltage RLD_VREF voltage in order to cope with higher DC offset. The bits rld_ref_sel_r change the RLD reference voltage to 0.7 V, 1.0 V and 1.49 V.

[Figure 23](#) shows the maximal electrode offset versus supply for different reference voltages.

Figure 23. Maximum DC offset removal

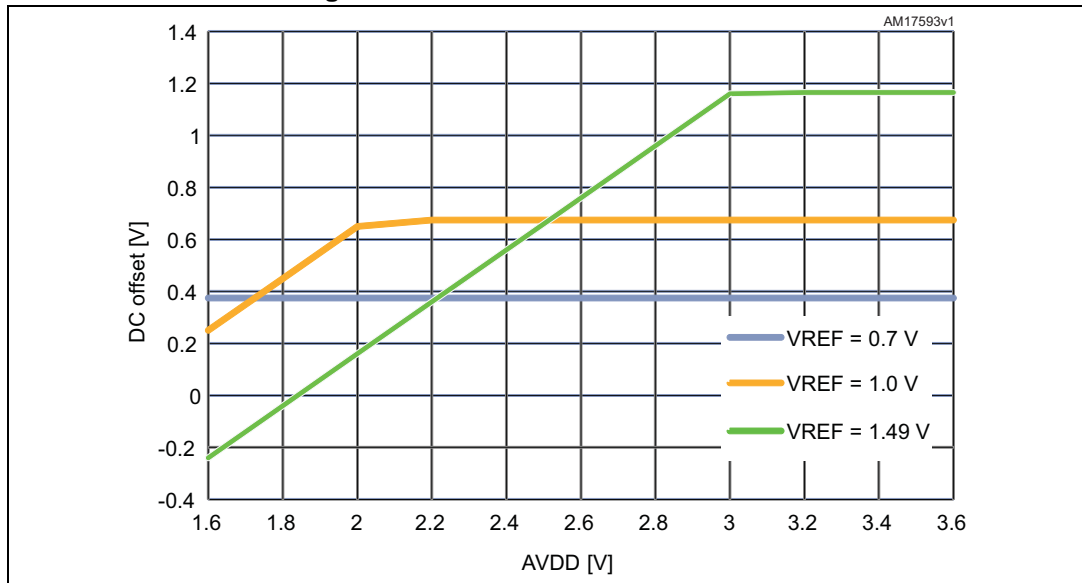

7.2 Multi-chip configuration


In order to build a system supporting more than 3 biopotential channels, the HM301D can be used in a multiple chip configuration.

In this configuration the SPI will be configured as daisy chained SPI by connecting the data output of one device to the data input of another. The first and the last devices of the chain will be connected to the MCU. The maximum number of devices that can be connected together is 4.

One of the HM301D chip can be used as analog master in the system: it distributes the WCT signal, drives the shield and right leg and sends out its clock signal to the others.

Figure 24 shows an example of 3 HM301D connected together for 12 leads ECG application.

Figure 24. Example of chain connection: standard 12-lead ECG

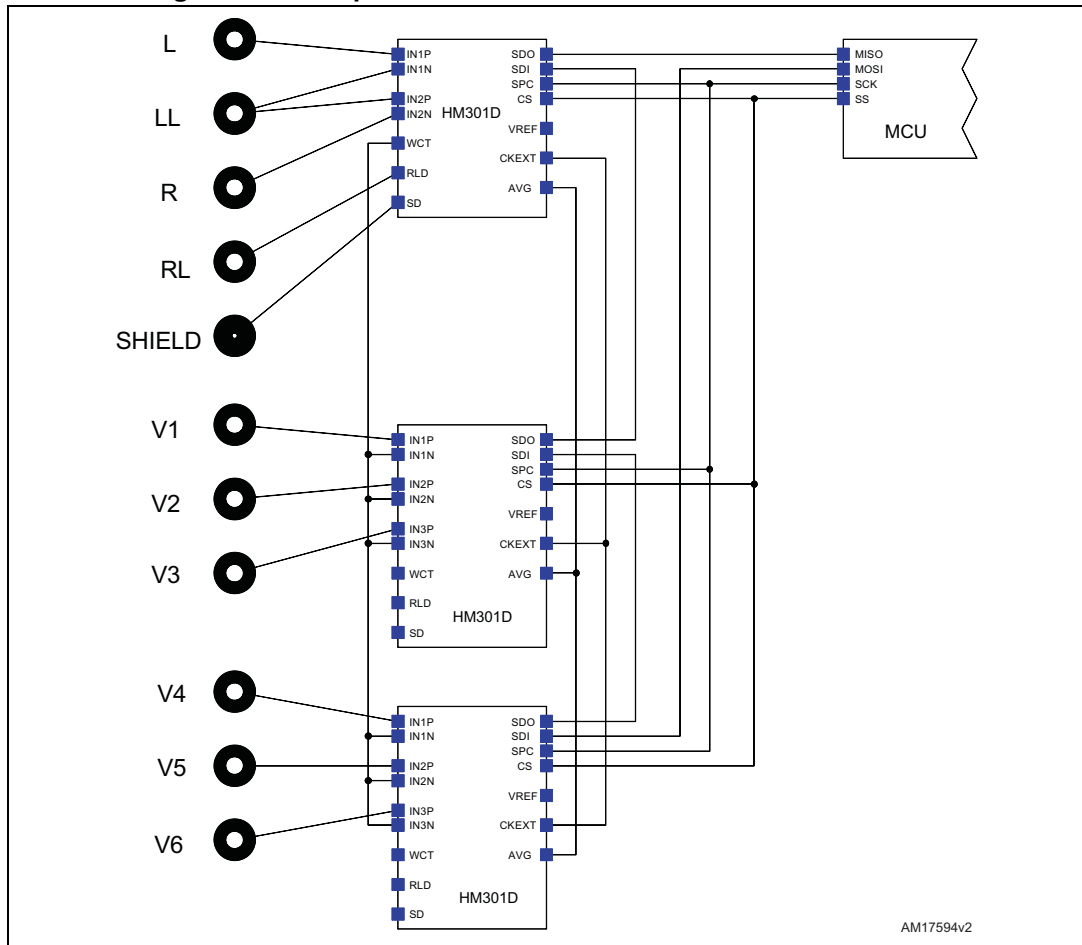

In multi-chip configuration the data send and received by the MCU through the SPI are formatted in a different way compared to single chip configuration.

7.3 Supported ECG configurations

Even if designed for any type of biopotential acquisition, the HM301D is particularly suited to ECG systems. To address most possible applications, each channel of the HM301D can be connected to the electrodes either as bipolar or unipolar.

Table 88. Common ECG configurations

Application	Electrodes	Connection	Channels	Device
Standards 12 leads ECG	9 + RL	2 Bipolar + 6 Unipolar	8	3x HM301D
Standards 12 leads ECG	9 + RL	9 Unipolar	9	3x HM301D
Interpolated 12 leads using a 6 wires cable	5 + RL	2 bipolar + 2 unipolar	4	2x HM301D
Interpolated 12 leads using a 6 wires cable	5 + RL	5 unipolar	5	2x HM301D
5 leads wire / EASI	4 + RL	2 bipolar + 1 unipolar	3	1x HM301D
5 leads wire / EASI	4 + RL	4 unipolar	4	2x HM301D
Einthoven's Triangle	3 + RL	2 bipolar	2	1x HM301D
Einthoven's Triangle	3 + RL	3 unipolar	2	1x HM301D
Rhythm	2	1 bipolar	1	1x HM301D
Automated External Defibrillator (AED)	2	1 bipolar	1	1x HM301D

At the output of the channel, the bipolar configuration gives the difference between 2 electrodes. Otherwise, the unipolar configuration reads the difference between the single electrode voltage and a reference voltage (the internal reference or WCT from the same chip or from the master chip in a chain connection).

As an example the standard 12-lead electrocardiogram application is shown in [Figure 24](#). It requires the measurement of 12 differential signals, exploiting 9 electrodes. 8 differential channels are obtained by cascading 3 HM301D. The master (IC in the top) is connected to the 3 limb electrodes using a bipolar connection for both channels. It provides a WCT signal, clock timing and drives the RL electrode. HM301D devices, configured as unipolar, measure all 6 chest electrodes with respect to WCT. Combining the resulting 8 outputs, all 12 standards leads can be evaluated.

8 Package mechanical data

In order to meet environmental requirements, ST offers these devices in different grades of ECOPACK[®] packages, depending on their level of environmental compliance. ECOPACK[®] specifications, grade definitions and product status are available at: www.st.com. ECOPACK[®] is an ST trademark.

Figure 25. Package outline for LGA 40L (6 x 6 mm)

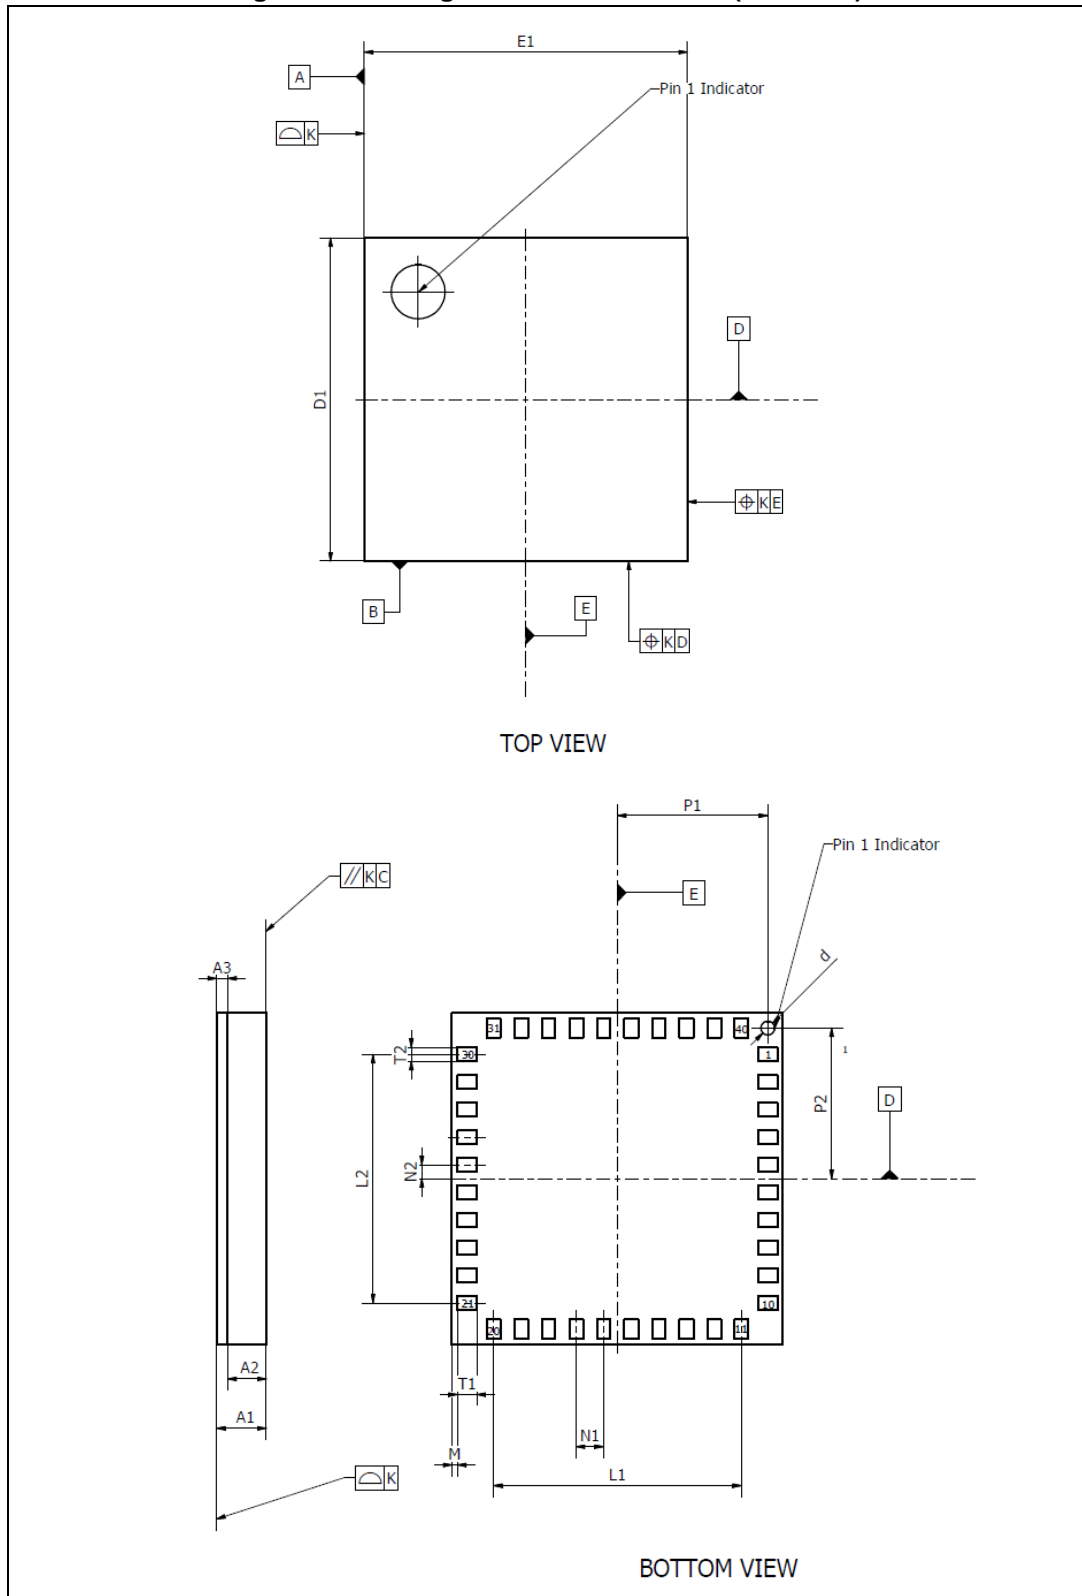


Table 89. LGA 40L (6 x 6 mm) mechanical data

Symbol	(mm)		
	Min.	Typ.	Max.
A1	0.810	0.900	0.960
A2	0.660	0.700	0.710
A3	0.150	0.200	0.250
D1	5.850	6.000	6150
E1	5.850	6.000	6150
L1	4.460	4.500	4.540
L2	4.460	4.500	4.540
N1	0.460	0.500	0.540
N2	0.210	0.250	0.290
M	0.060	0.100	0.140
P1	2.690	2.730	2.77
P2	2.690	2.730	2.77
T1	0.310	0.350	0.390
T2	0.310	0.350	0.390
d	0.210	0.250	0.290
K		0.050	

9 Revision history

Table 90. Document revision history

Date	Revision	Changes
01-Apr-2014	1	Initial release
11-Apr-2014	2	Updated order code Table 1 on page 1
14-May-2014	3	Changed unit ODR parameter Table 5 on page 12
01-Jul-2014	4	Updated name Table 58 on page 63

Please Read Carefully:

Information in this document is provided solely in connection with ST products. STMicroelectronics NV and its subsidiaries ("ST") reserve the right to make changes, corrections, modifications or improvements, to this document, and the products and services described herein at any time, without notice.

All ST products are sold pursuant to ST's terms and conditions of sale.

Purchasers are solely responsible for the choice, selection and use of the ST products and services described herein, and ST assumes no liability whatsoever relating to the choice, selection or use of the ST products and services described herein.

No license, express or implied, by estoppel or otherwise, to any intellectual property rights is granted under this document. If any part of this document refers to any third party products or services it shall not be deemed a license grant by ST for the use of such third party products or services, or any intellectual property contained therein or considered as a warranty covering the use in any manner whatsoever of such third party products or services or any intellectual property contained therein.

UNLESS OTHERWISE SET FORTH IN ST'S TERMS AND CONDITIONS OF SALE ST DISCLAIMS ANY EXPRESS OR IMPLIED WARRANTY WITH RESPECT TO THE USE AND/OR SALE OF ST PRODUCTS INCLUDING WITHOUT LIMITATION IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE (AND THEIR EQUIVALENTS UNDER THE LAWS OF ANY JURISDICTION), OR INFRINGEMENT OF ANY PATENT, COPYRIGHT OR OTHER INTELLECTUAL PROPERTY RIGHT.

ST PRODUCTS ARE NOT DESIGNED OR AUTHORIZED FOR USE IN: (A) SAFETY CRITICAL APPLICATIONS SUCH AS LIFE SUPPORTING, ACTIVE IMPLANTED DEVICES OR SYSTEMS WITH PRODUCT FUNCTIONAL SAFETY REQUIREMENTS; (B) AERONAUTIC APPLICATIONS; (C) AUTOMOTIVE APPLICATIONS OR ENVIRONMENTS, AND/OR (D) AEROSPACE APPLICATIONS OR ENVIRONMENTS. WHERE ST PRODUCTS ARE NOT DESIGNED FOR SUCH USE, THE PURCHASER SHALL USE PRODUCTS AT PURCHASER'S SOLE RISK, EVEN IF ST HAS BEEN INFORMED IN WRITING OF SUCH USAGE, UNLESS A PRODUCT IS EXPRESSLY DESIGNATED BY ST AS BEING INTENDED FOR "AUTOMOTIVE, AUTOMOTIVE SAFETY OR MEDICAL" INDUSTRY DOMAINS ACCORDING TO ST PRODUCT DESIGN SPECIFICATIONS. PRODUCTS FORMALLY ESCC, QML OR JAN QUALIFIED ARE DEEMED SUITABLE FOR USE IN AEROSPACE BY THE CORRESPONDING GOVERNMENTAL AGENCY.

Resale of ST products with provisions different from the statements and/or technical features set forth in this document shall immediately void any warranty granted by ST for the ST product or service described herein and shall not create or extend in any manner whatsoever, any liability of ST.

ST and the ST logo are trademarks or registered trademarks of ST in various countries.

Information in this document supersedes and replaces all information previously supplied.

The ST logo is a registered trademark of STMicroelectronics. All other names are the property of their respective owners.

© 2014 STMicroelectronics - All rights reserved

STMicroelectronics group of companies

Australia - Belgium - Brazil - Canada - China - Czech Republic - Finland - France - Germany - Hong Kong - India - Israel - Italy - Japan - Malaysia - Malta - Morocco - Philippines - Singapore - Spain - Sweden - Switzerland - United Kingdom - United States of America

www.st.com

